

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 05/15/2014

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14040

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:28
INTERNAL STANDARD	VERIFIED	04:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	04:28
BLANK TEST	0.00	04:29
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	04:29
BLANK TEST	0.00	04:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	04:31
BLANK TEST	0.00	04:31

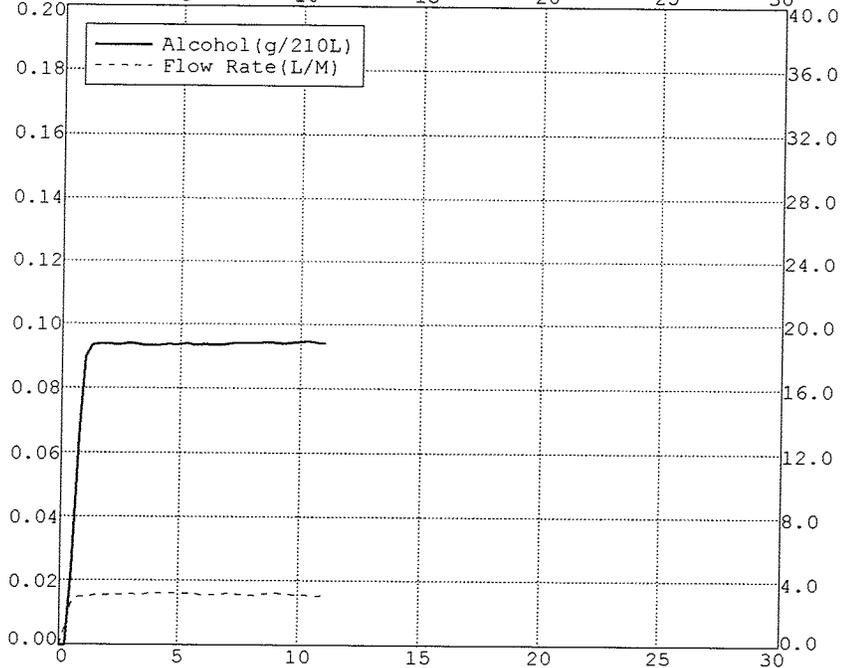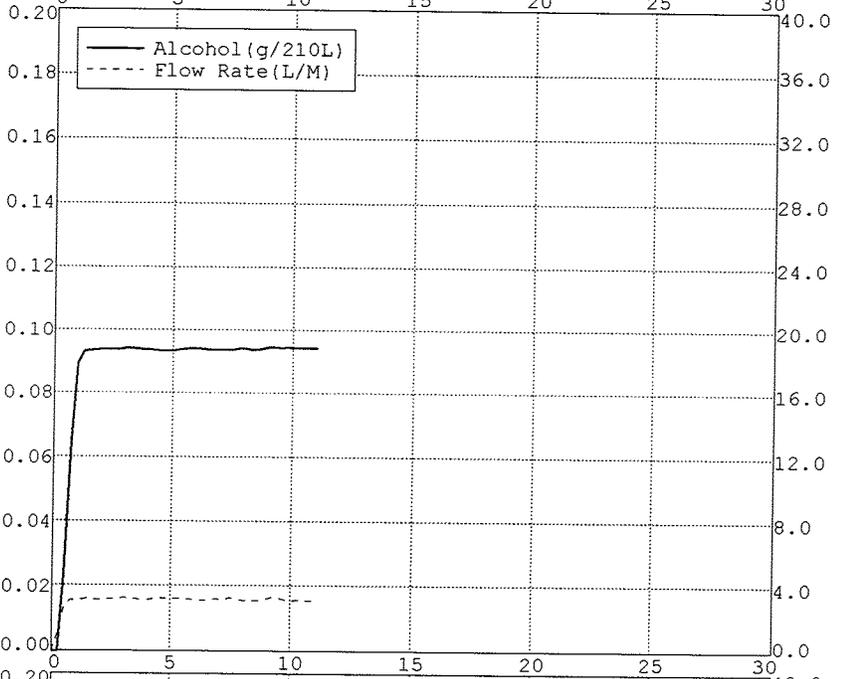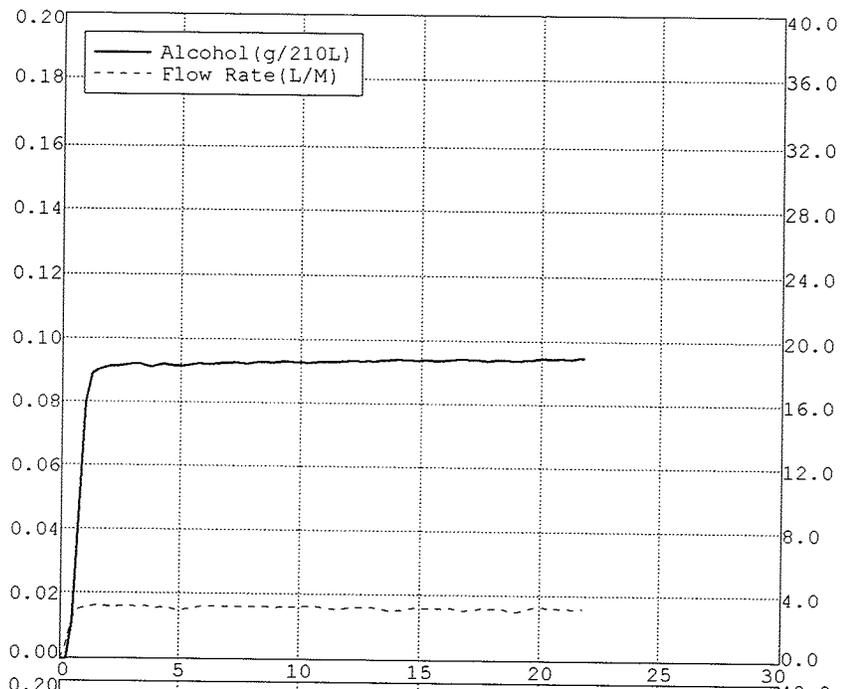

SGS Rpt by Thomas WSC #162 05-15-14