

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 05/26/2014

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14040

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:09
INTERNAL STANDARD	VERIFIED	05:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:09
BLANK TEST	0.00	05:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:11
BLANK TEST	0.00	05:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	05:12
BLANK TEST	0.00	05:13

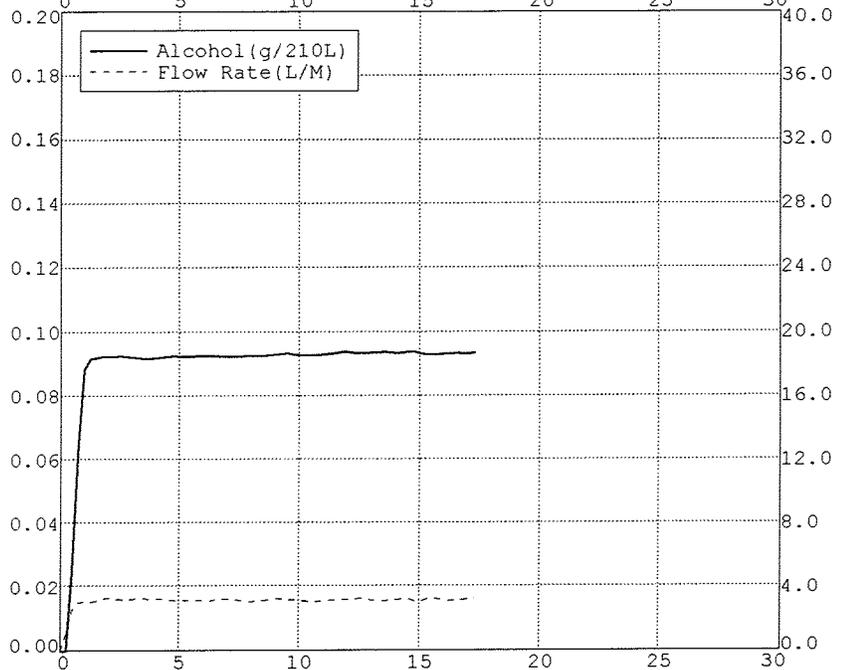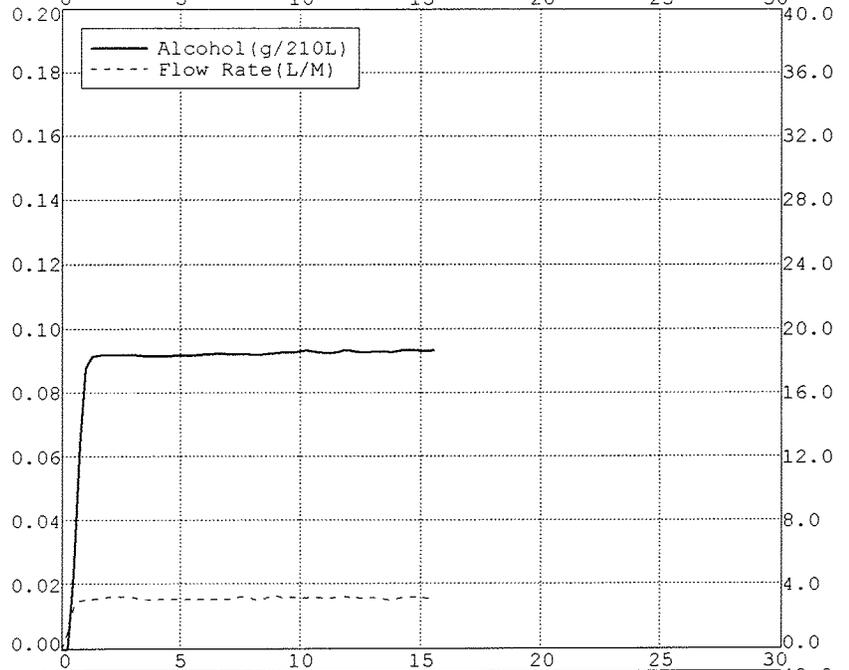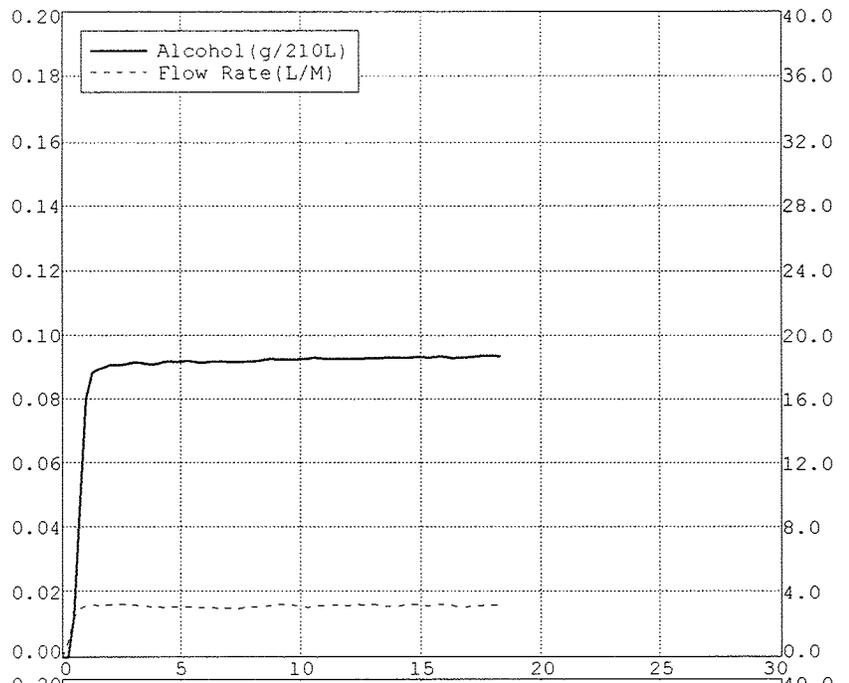

505 RJA Bartlett weso#162

05-26-14