

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 06/09/2014

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14080

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:14
INTERNAL STANDARD	VERIFIED	00:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	00:15
BLANK TEST	0.00	00:16
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	00:16
BLANK TEST	0.00	00:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	00:17
BLANK TEST	0.00	00:18

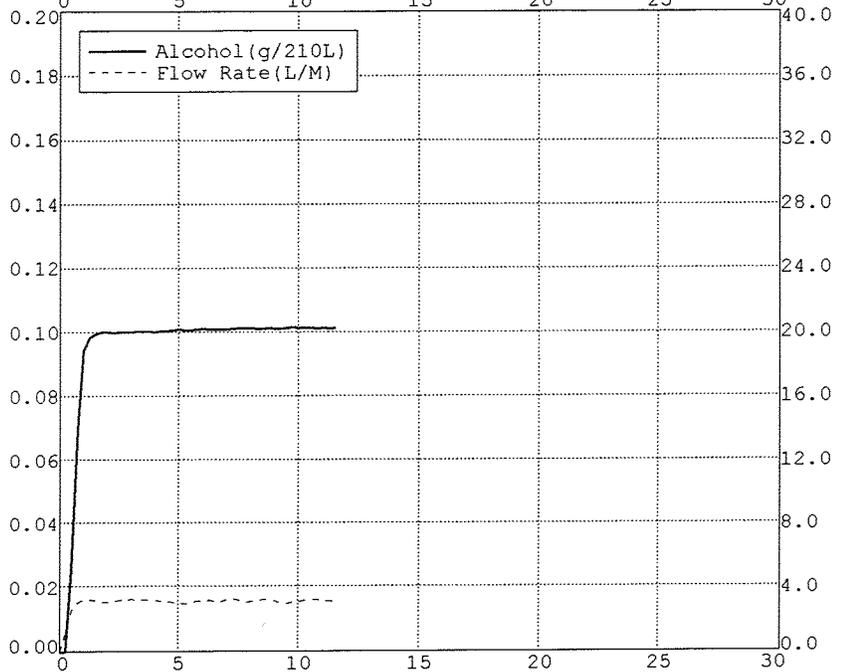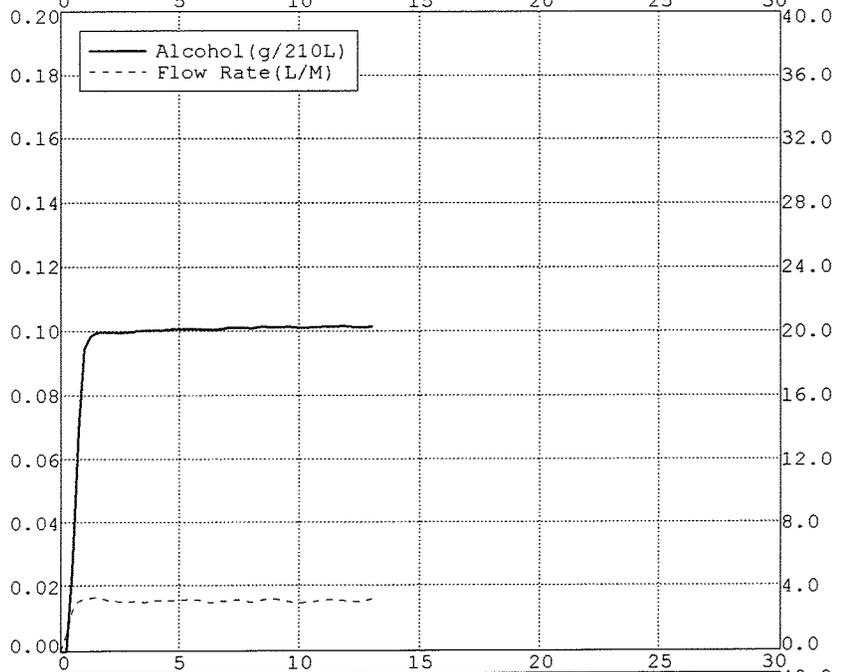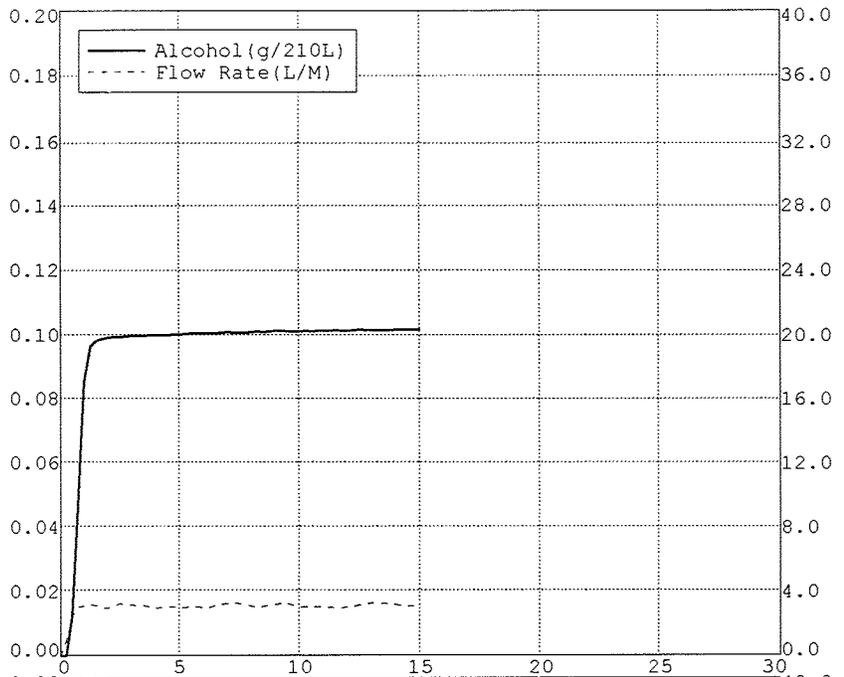

SGT Ralph J Bartlett WCSO #162

06-09-14