

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 06/17/2014

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 14080

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:59
INTERNAL STANDARD	VERIFIED	03:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:00
BLANK TEST	0.00	03:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:01
BLANK TEST	0.00	03:02
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:03
BLANK TEST	0.00	03:03

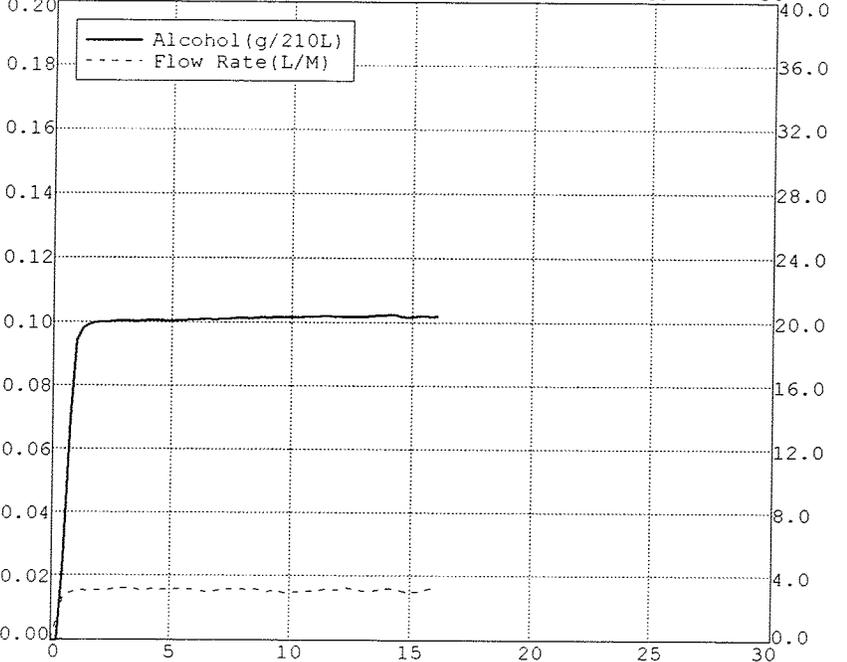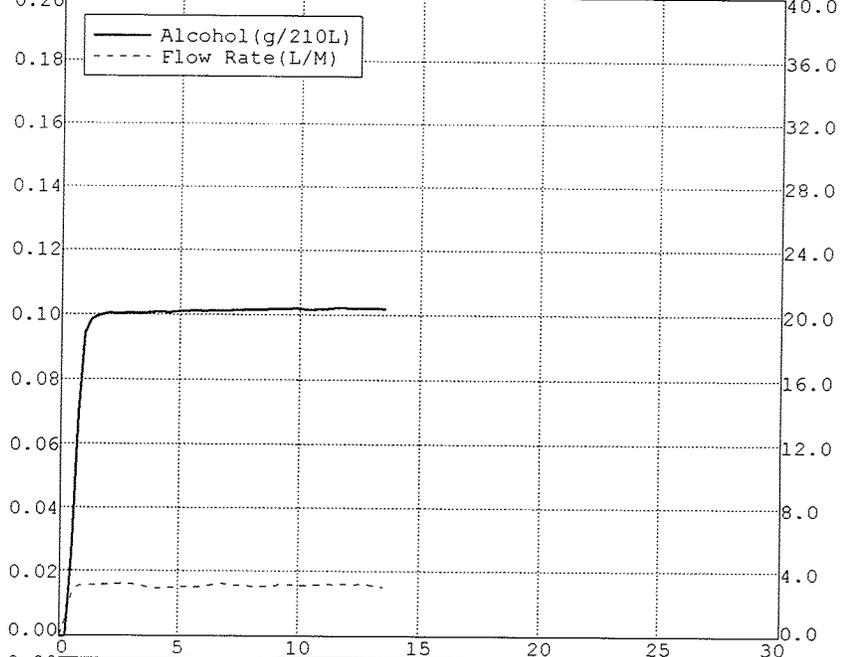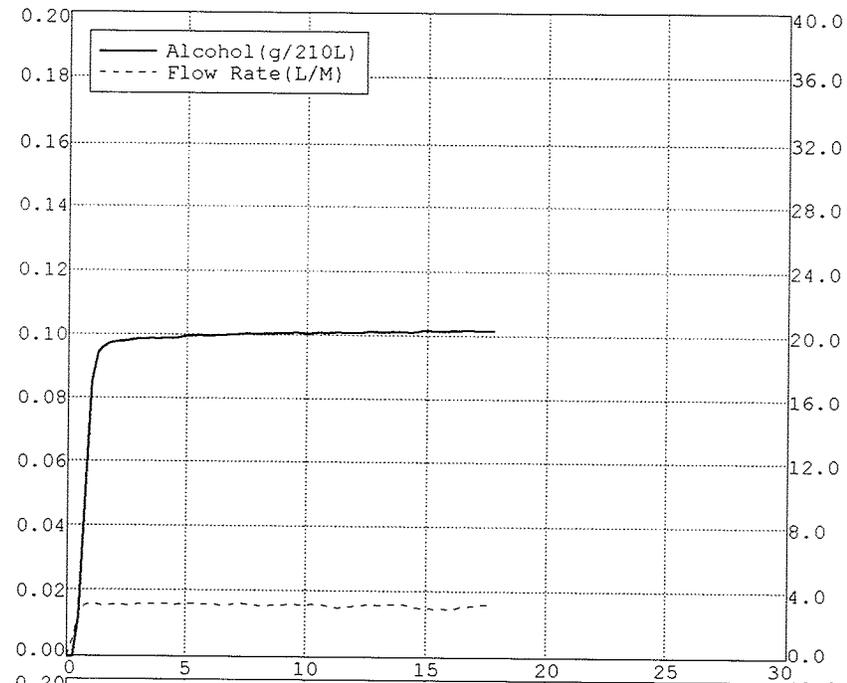

*505 R/L J Bartlett*

WCSD #102 06-17-14