

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 06/23/2014

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14080

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:31
INTERNAL STANDARD	VERIFIED	02:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:31
BLANK TEST	0.00	02:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	02:33
BLANK TEST	0.00	02:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	02:34
BLANK TEST	0.00	02:35

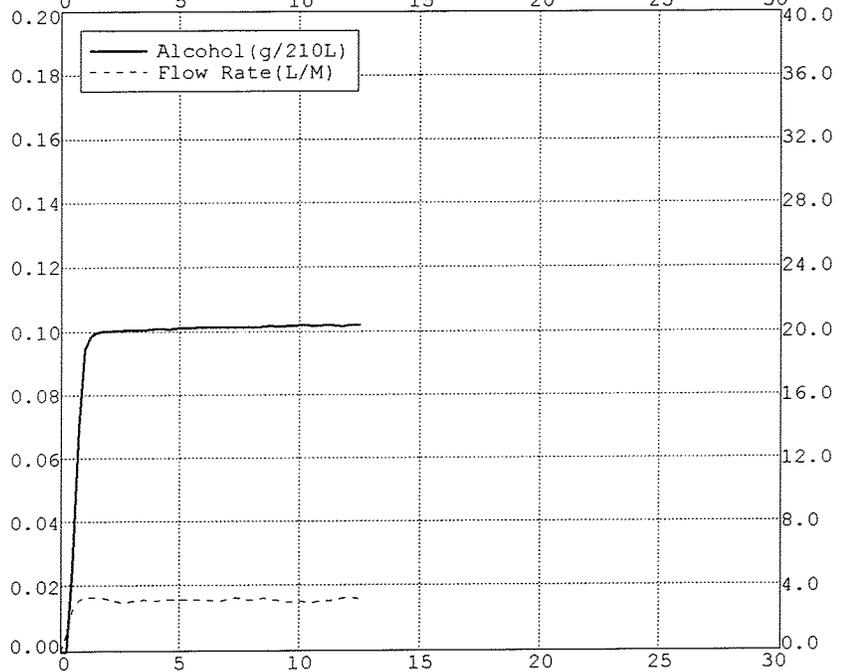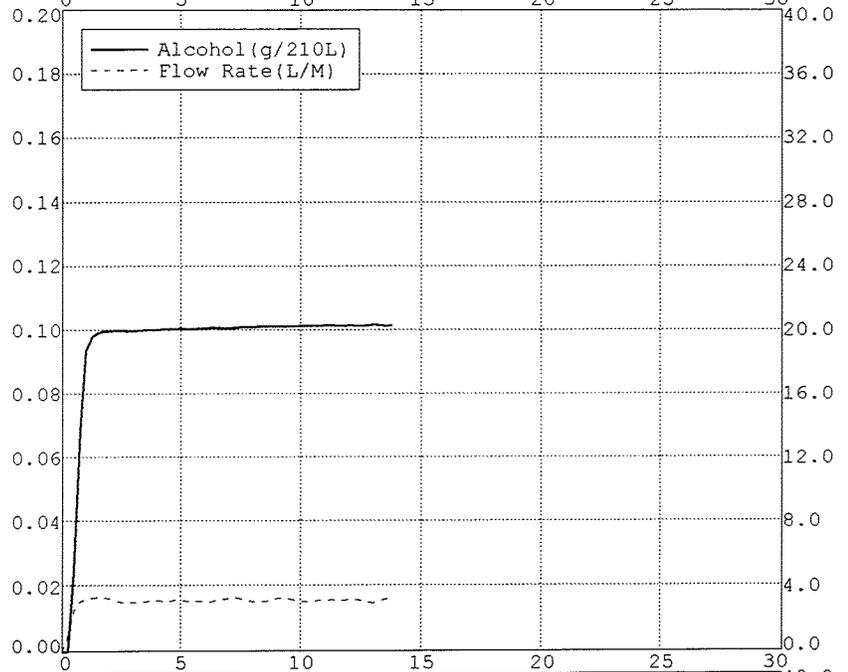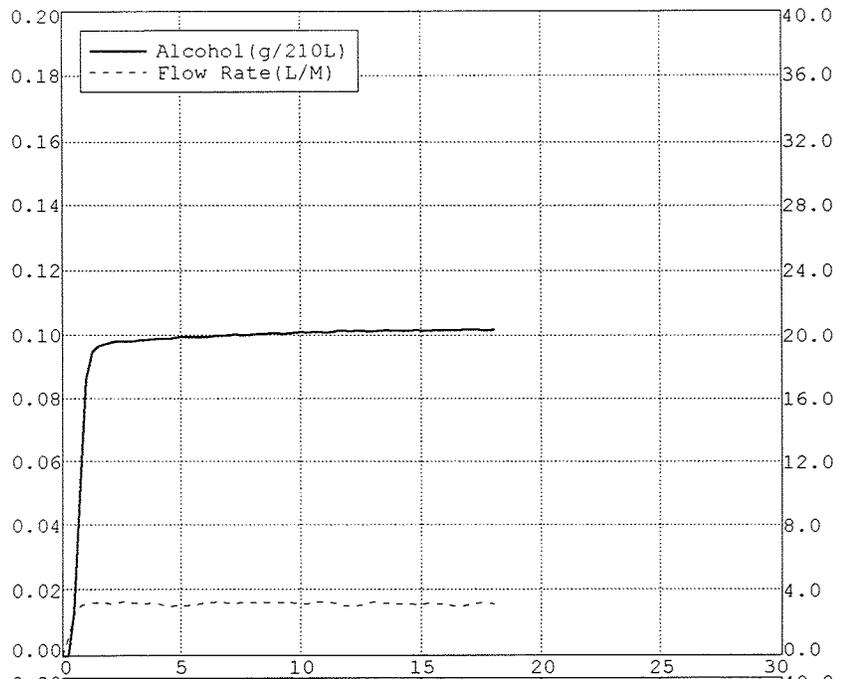

SGT R.J. Bartlett WSP #162
06-23-14