

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 07/21/2014

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 14080

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:45
INTERNAL STANDARD	VERIFIED	18:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:46
BLANK TEST	0.00	18:47
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	18:47
BLANK TEST	0.00	18:48
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:48
BLANK TEST	0.00	18:49

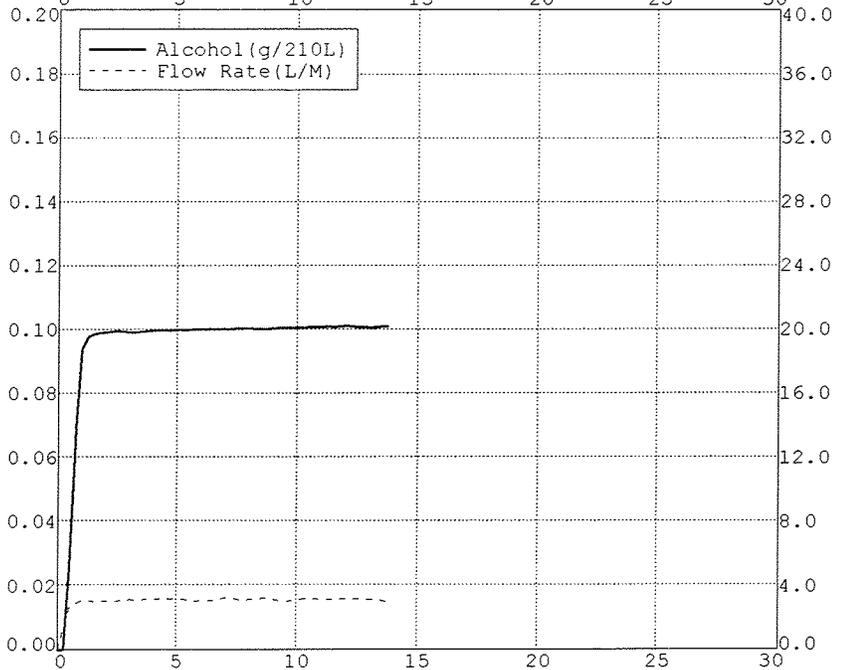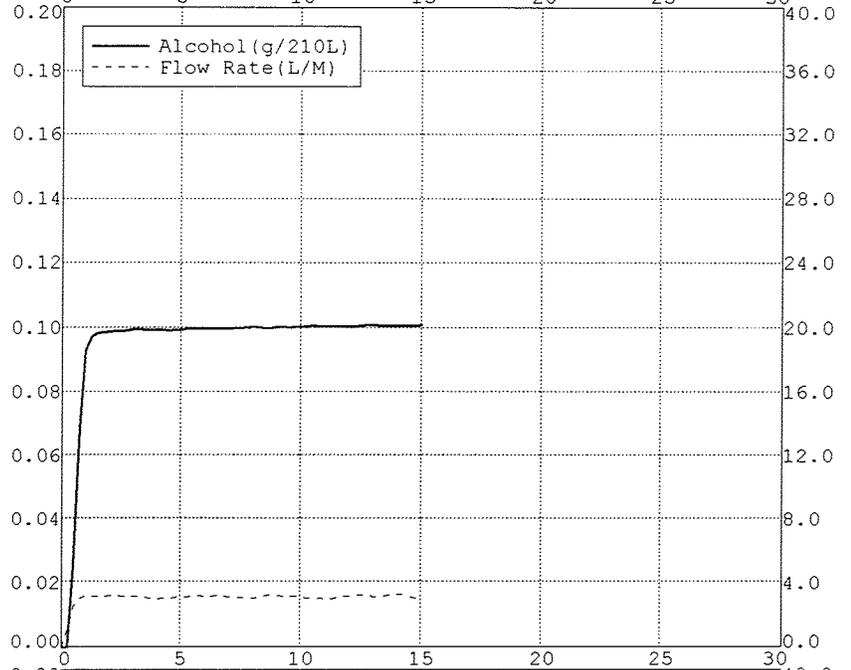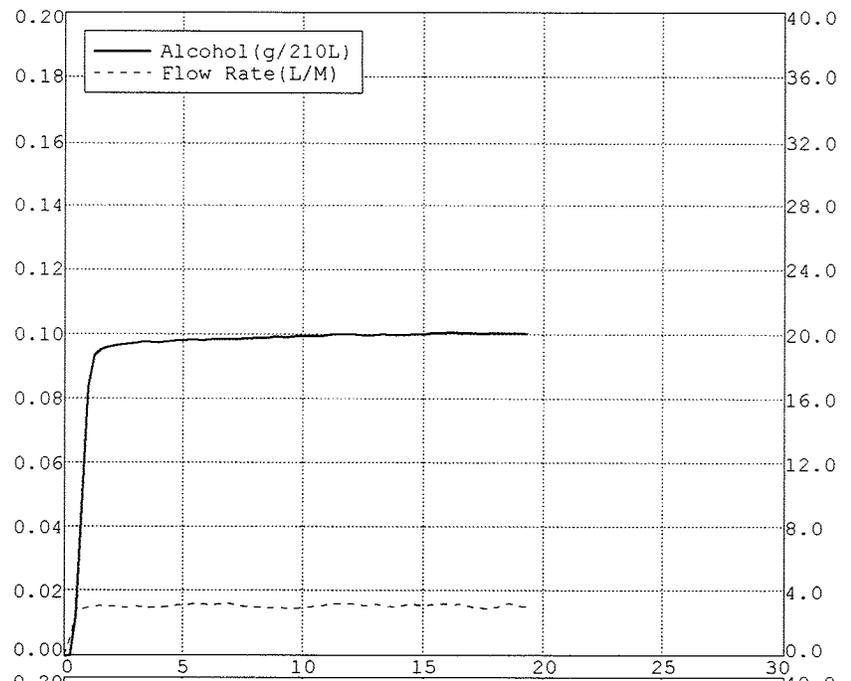

Charles B. Geisler
 7/21/14 1850