

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 09/01/2014

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14140

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:56
INTERNAL STANDARD	VERIFIED	01:56
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	01:56
BLANK TEST	0.00	01:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:57
BLANK TEST	0.00	01:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:59
BLANK TEST	0.00	01:59

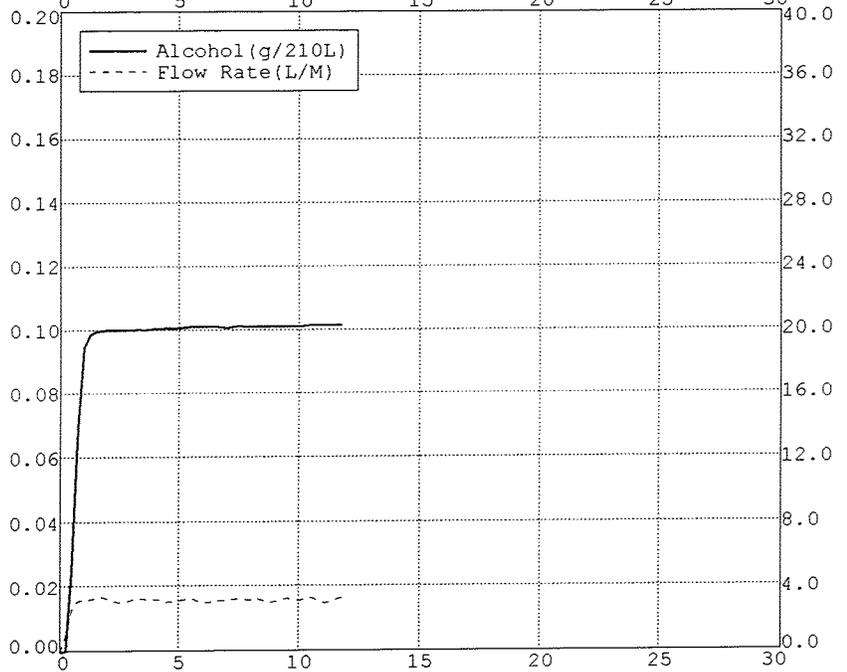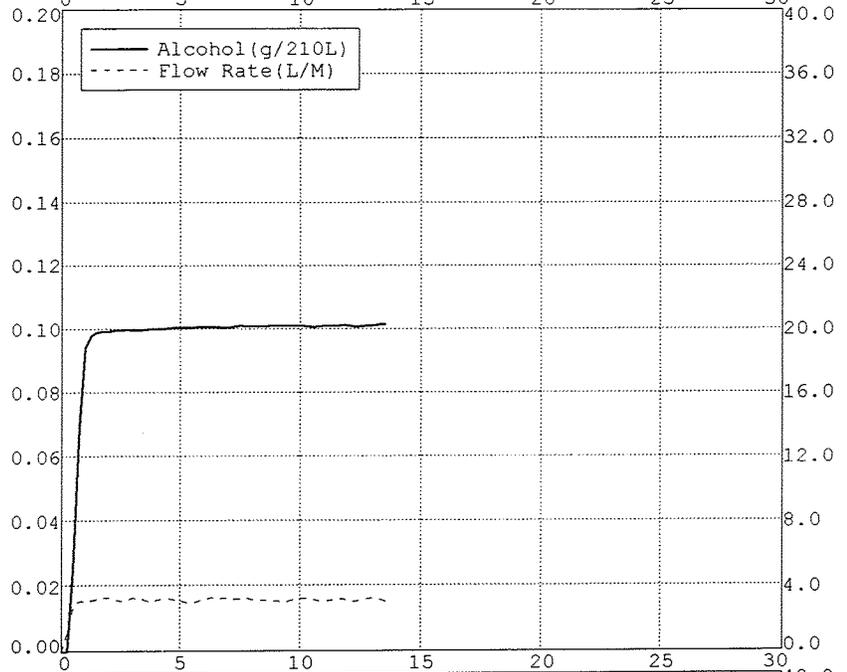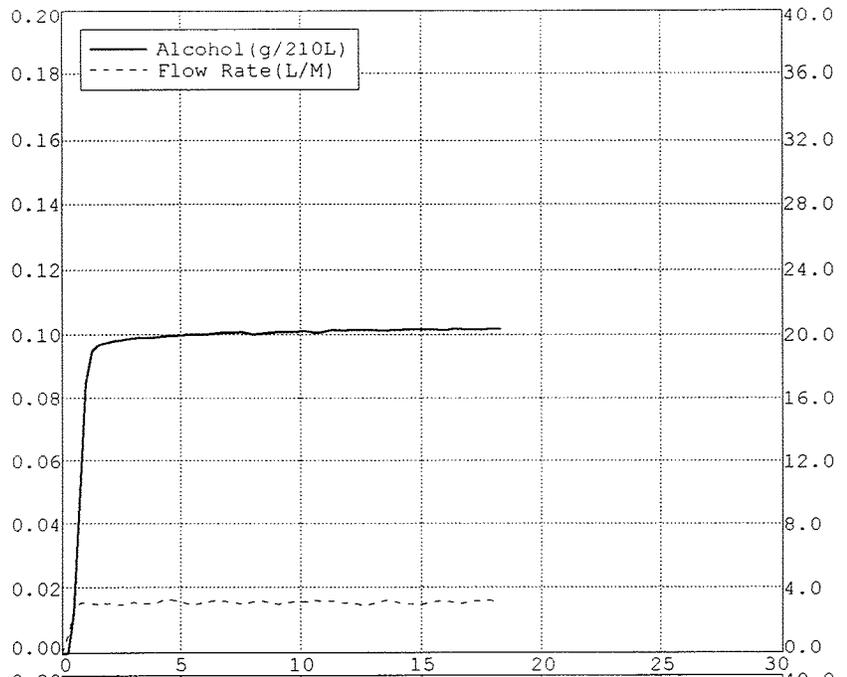

SGT RJA [Signature] #162

09-01-14