

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 09/15/2014

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 14140

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:50
INTERNAL STANDARD	VERIFIED	02:50
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	02:50
BLANK TEST	0.00	02:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	02:51
BLANK TEST	0.00	02:52
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	02:53
BLANK TEST	0.00	02:54

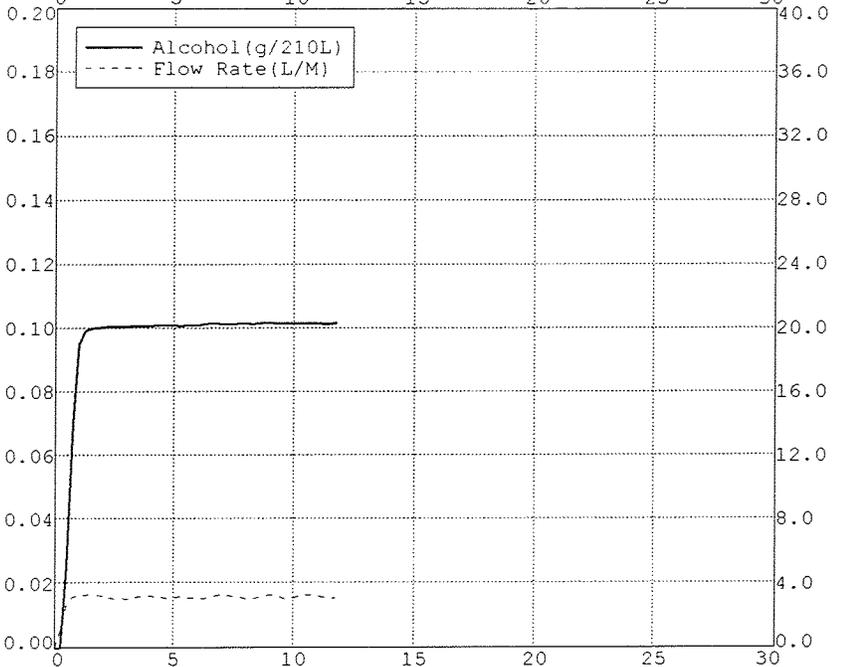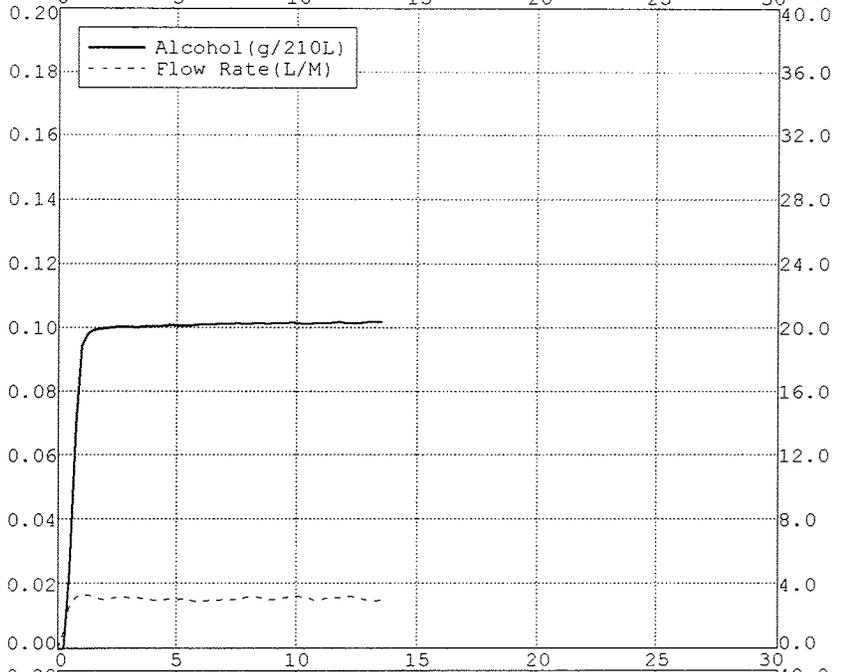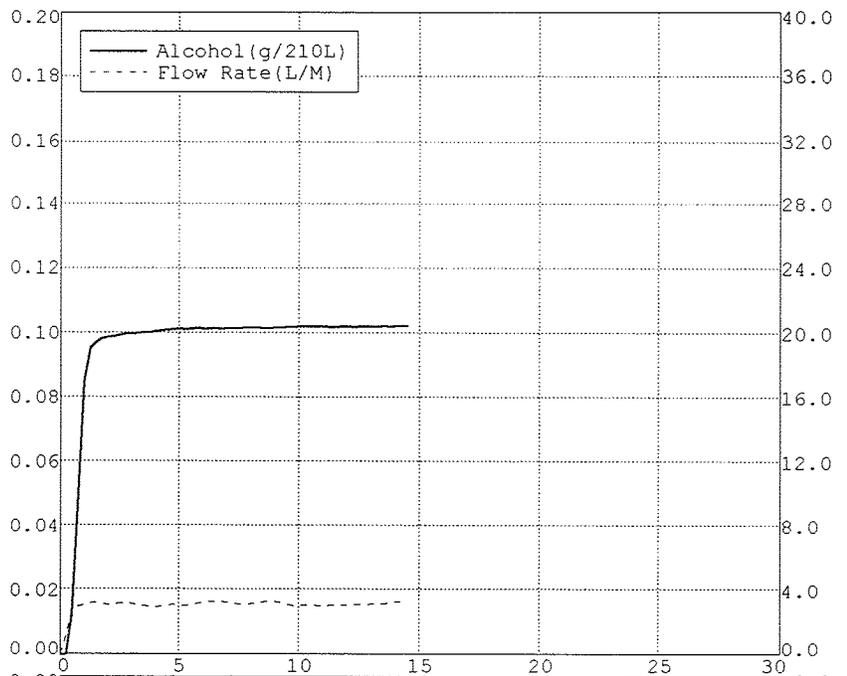

SG: *RJ Bartlett* weso #16c  
09-15-14