

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 09/23/2014

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14140

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:45
INTERNAL STANDARD	VERIFIED	02:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	02:46
BLANK TEST	0.00	02:47
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	02:47
BLANK TEST	0.00	02:48
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	02:48
BLANK TEST	0.00	02:49

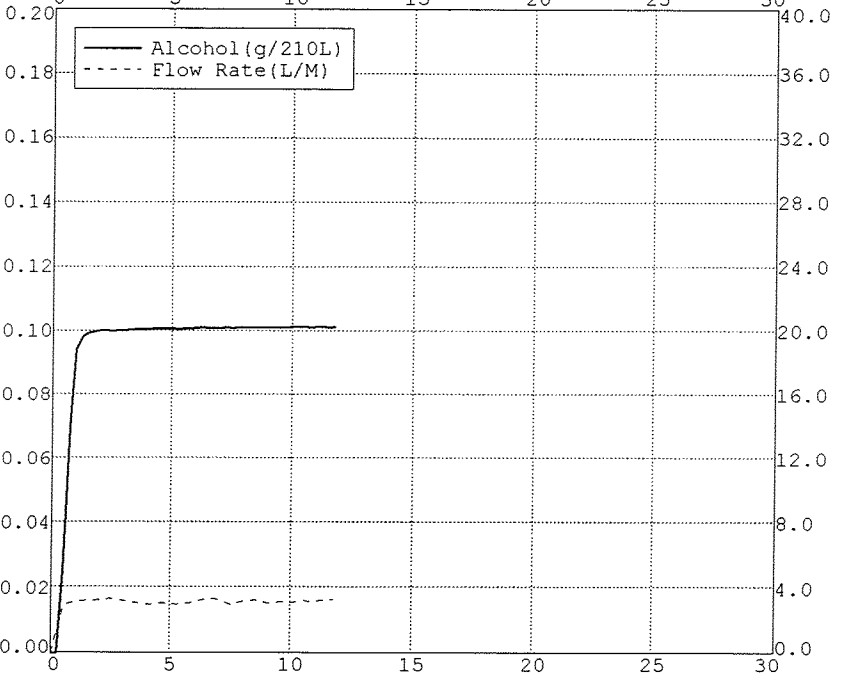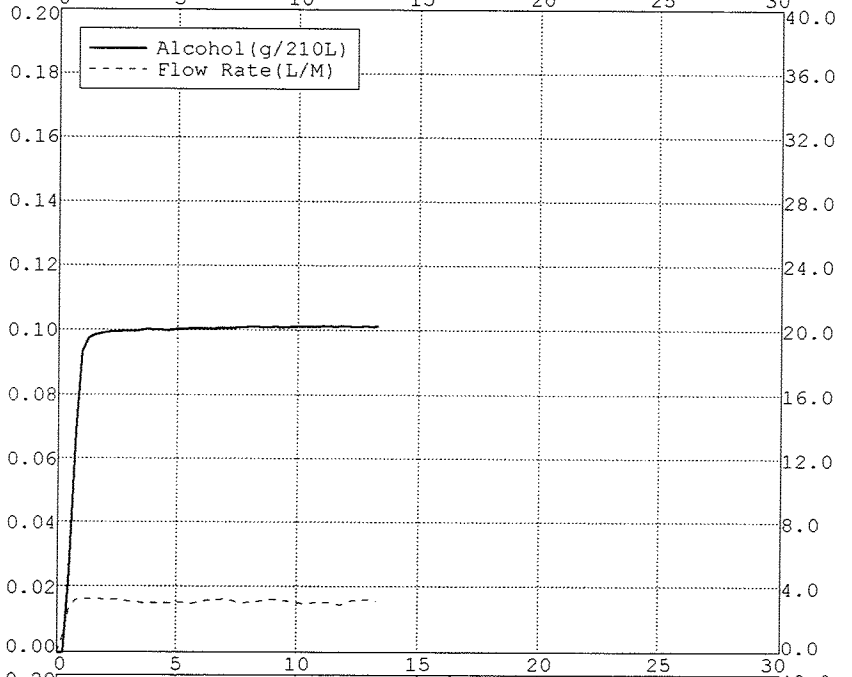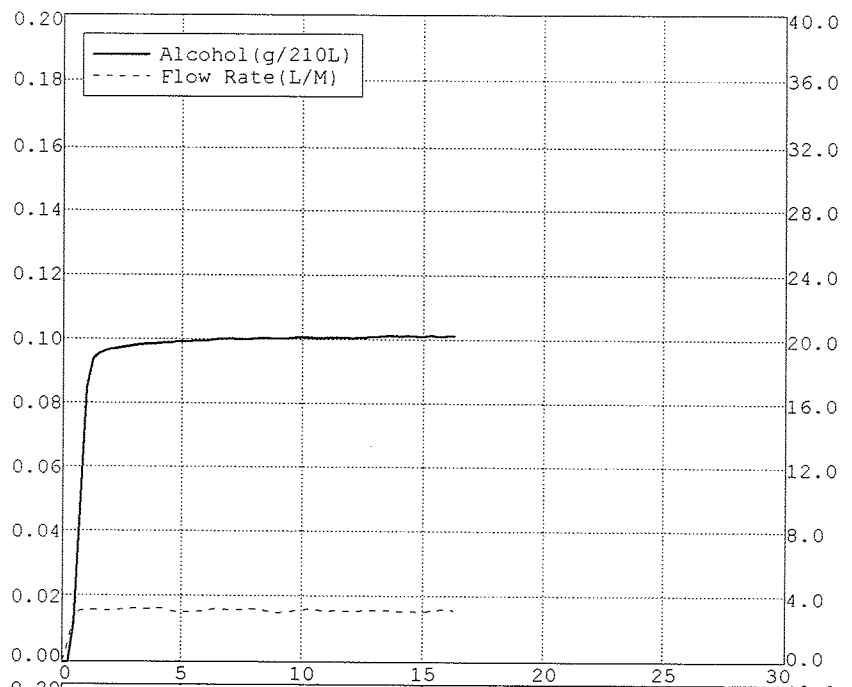

Sgt R J Bartlett WCSO #102
09-23-14