

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 09/29/2014

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14180

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 05:15 |
| INTERNAL STANDARD | VERIFIED | 05:15 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 05:16 |
| BLANK TEST | 0.00 | 05:17 |
| REFERENCE STANDARD TEMP | 34.02c | |
| REFERENCE STANDARD | 0.10 | 05:17 |
| BLANK TEST | 0.00 | 05:18 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 05:18 |
| BLANK TEST | 0.00 | 05:19 |

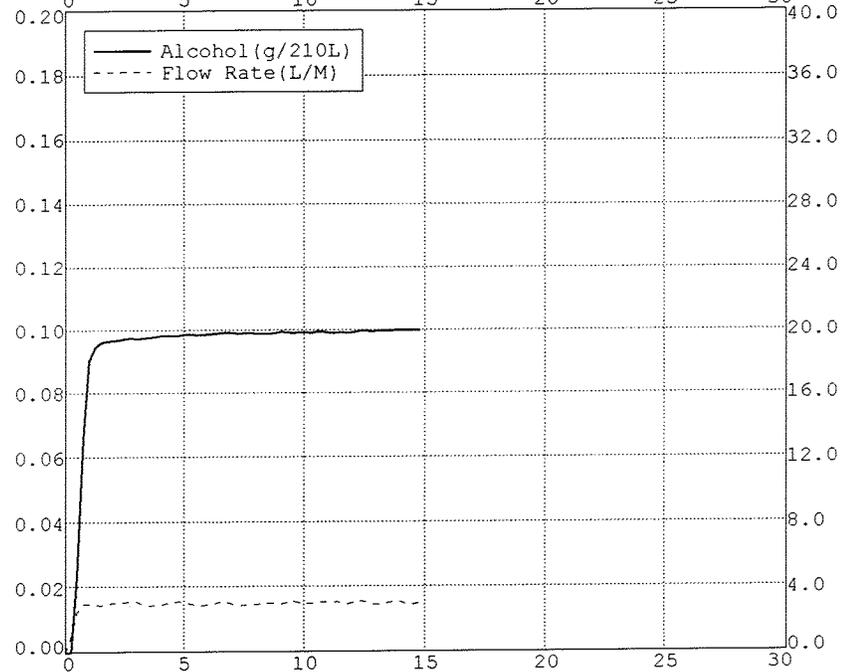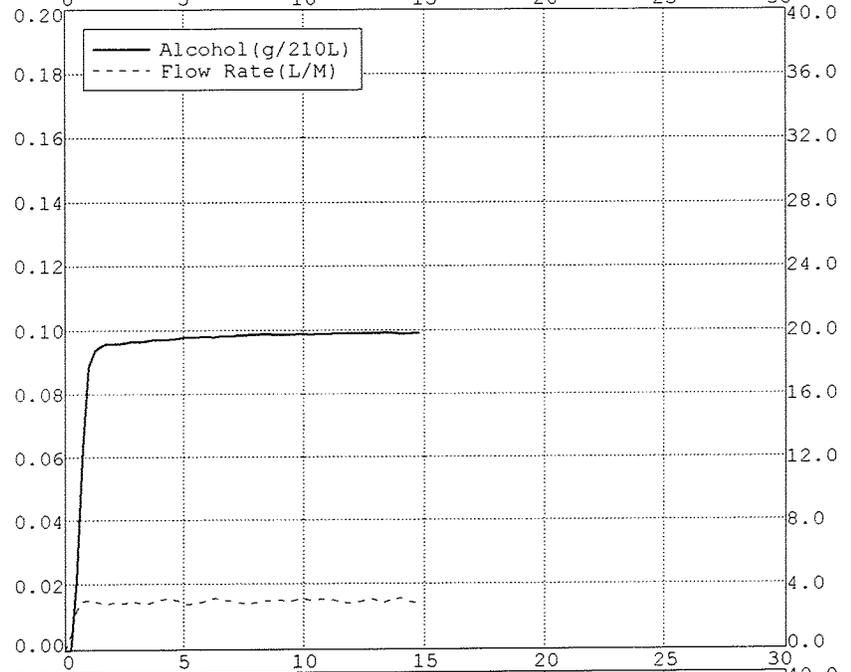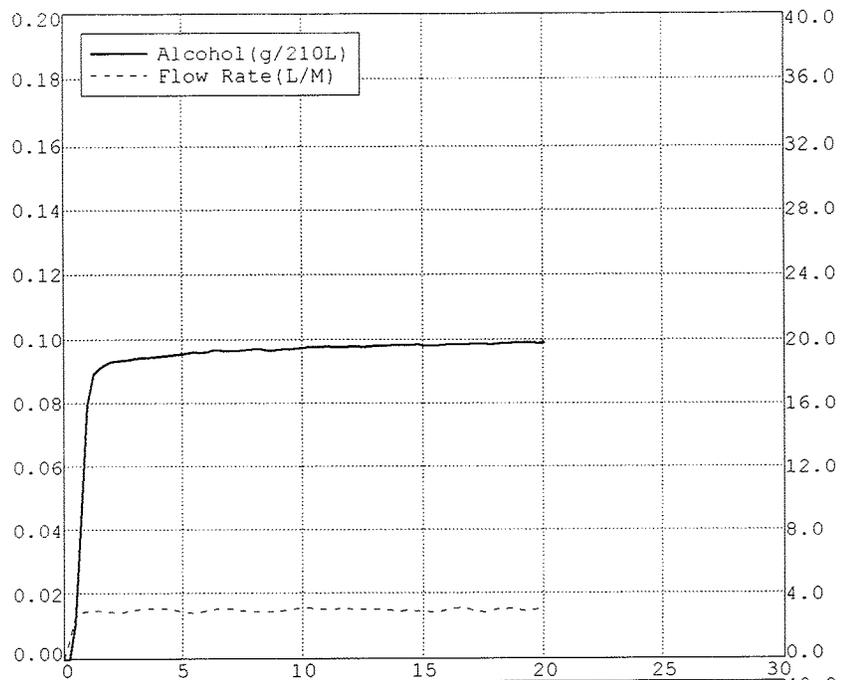

SGS Rky Dunton wase # 162
09-29-14