

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 10/15/2014

OPERATOR NAME:
KENNETH W SMITH
Permit #: 35604
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14180

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:35
INTERNAL STANDARD	VERIFIED	19:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:36
BLANK TEST	0.00	19:37
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	19:37
BLANK TEST	0.00	19:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:38
BLANK TEST	0.00	19:39

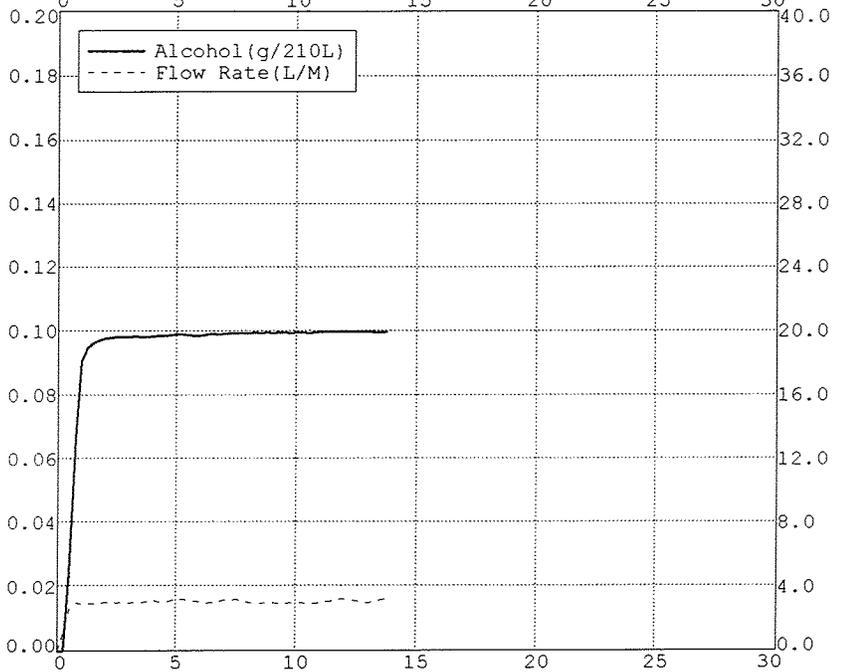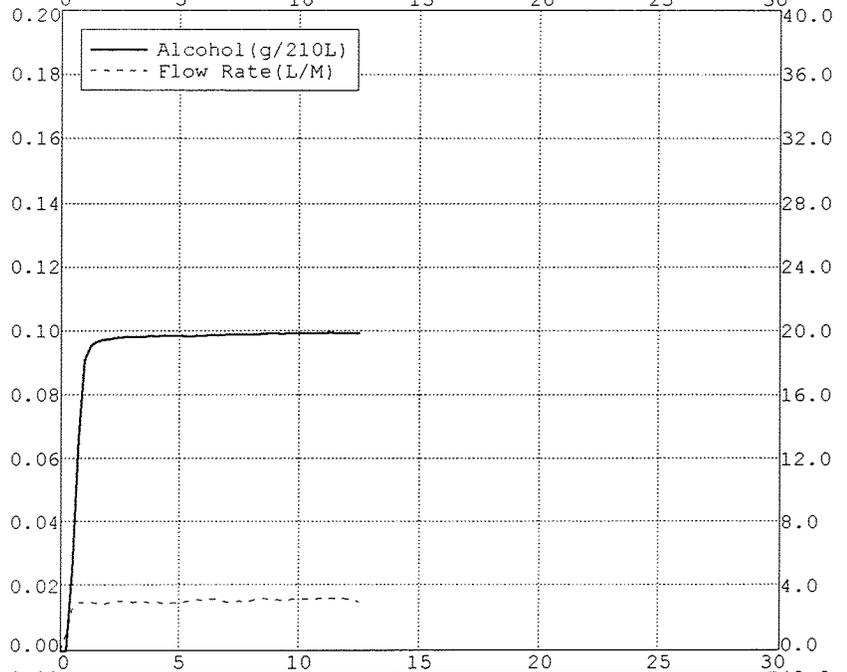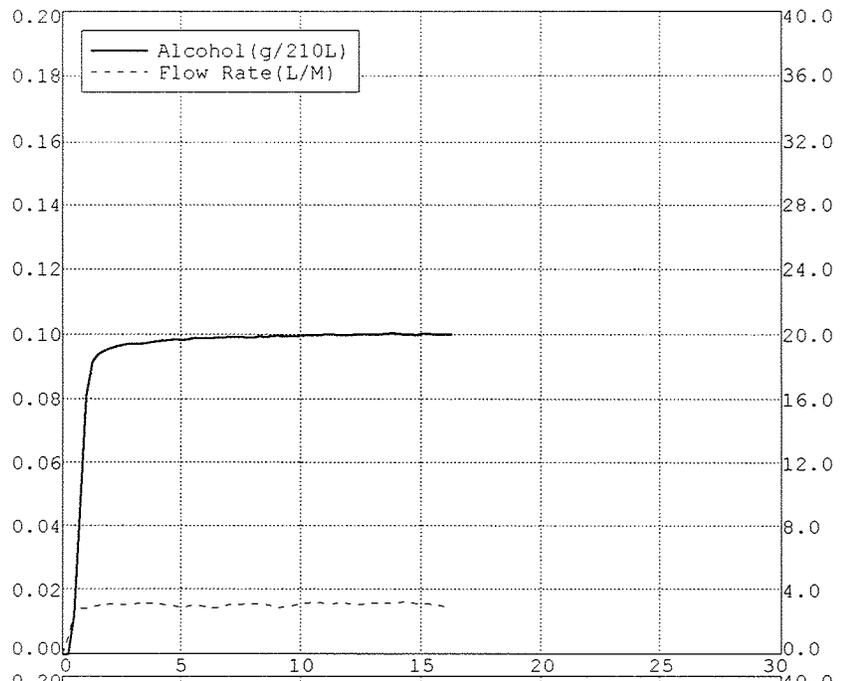

P.O. *[Signature]* #301
10/15/14