

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 10/21/2014

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14180

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:13
INTERNAL STANDARD	VERIFIED	02:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:14
BLANK TEST	0.00	02:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	02:15
BLANK TEST	0.00	02:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:16
BLANK TEST	0.00	02:17

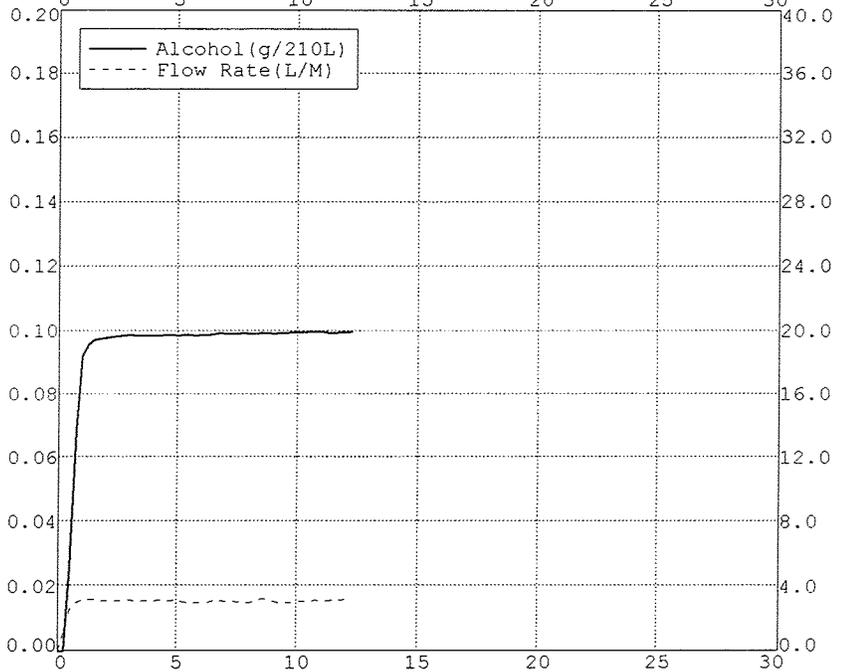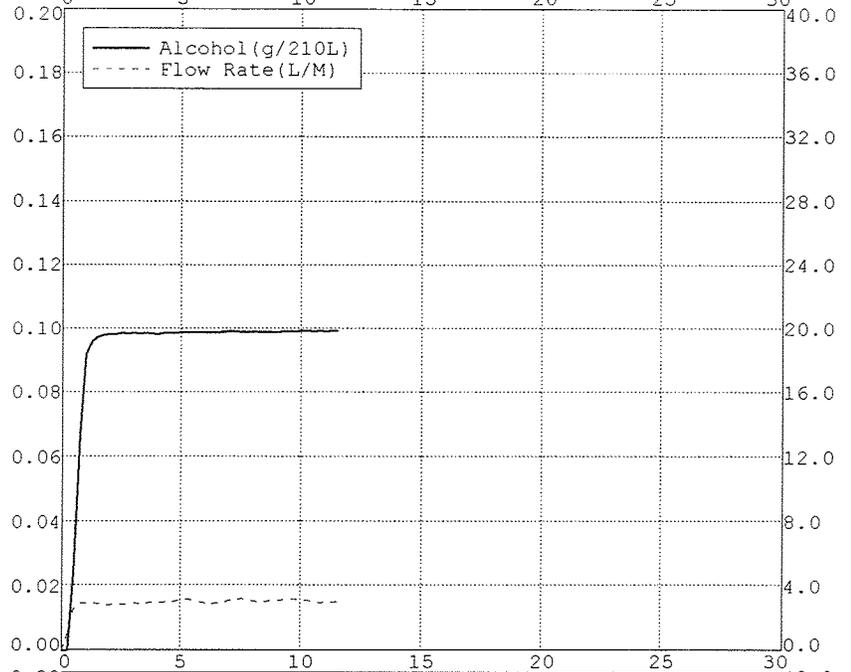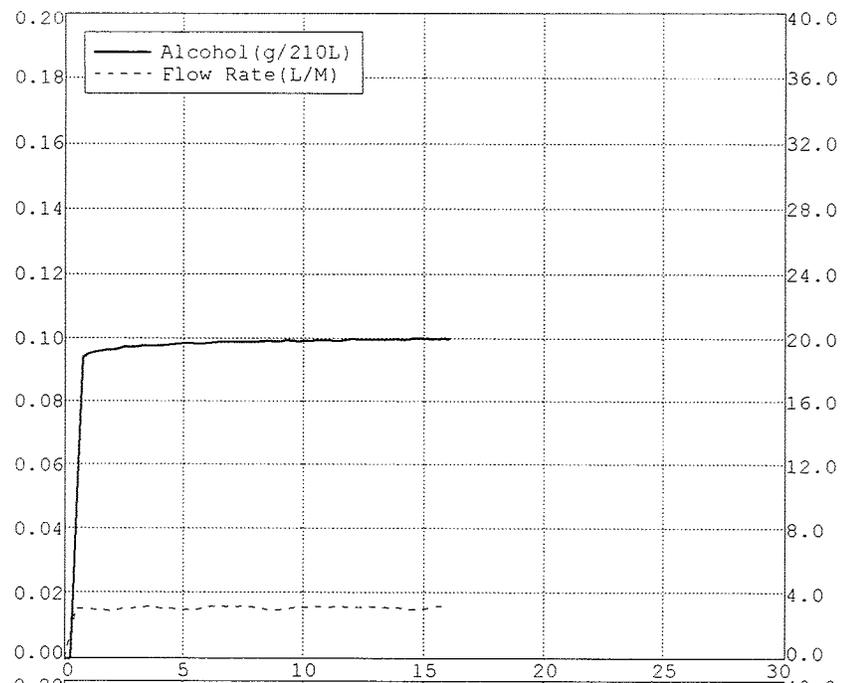

SOS RTJ Bartlett WOSO #162
10-21-14