

SUPERVISOR TEST



WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 11/10/2014

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 14180

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:20
INTERNAL STANDARD	VERIFIED	07:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:20
BLANK TEST	0.00	07:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:22
BLANK TEST	0.00	07:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:23
BLANK TEST	0.00	07:24

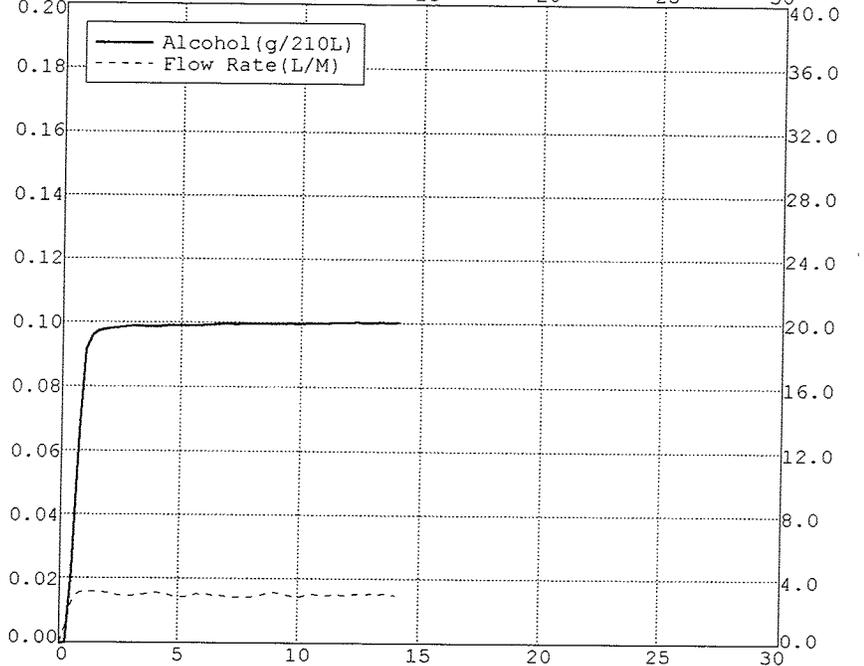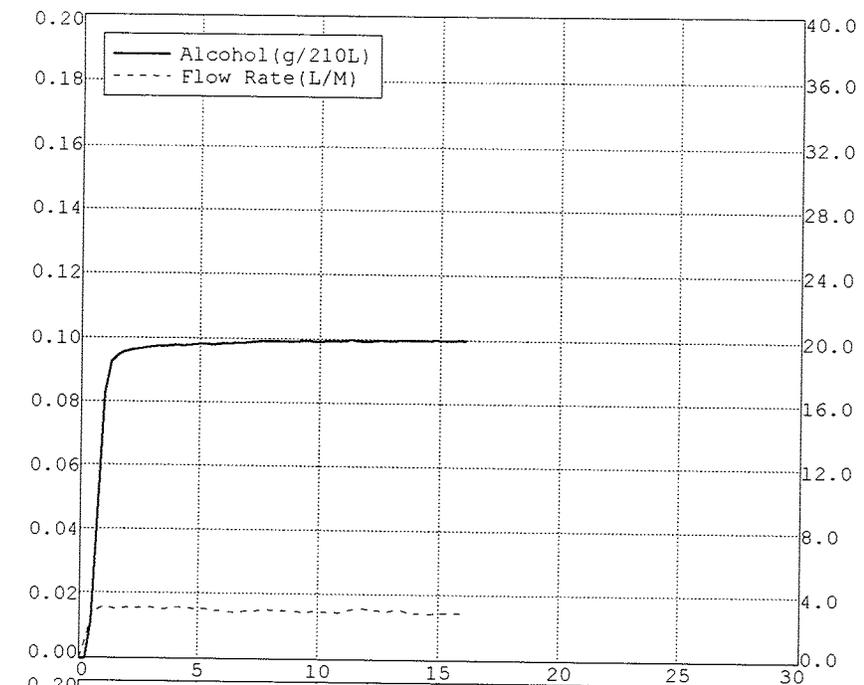

*Charles B. Geisler*