

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 11/16/2014

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 14180

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:34
INTERNAL STANDARD	VERIFIED	07:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:34
BLANK TEST	0.00	07:35
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	07:35
BLANK TEST	0.00	07:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:37
BLANK TEST	0.00	07:37

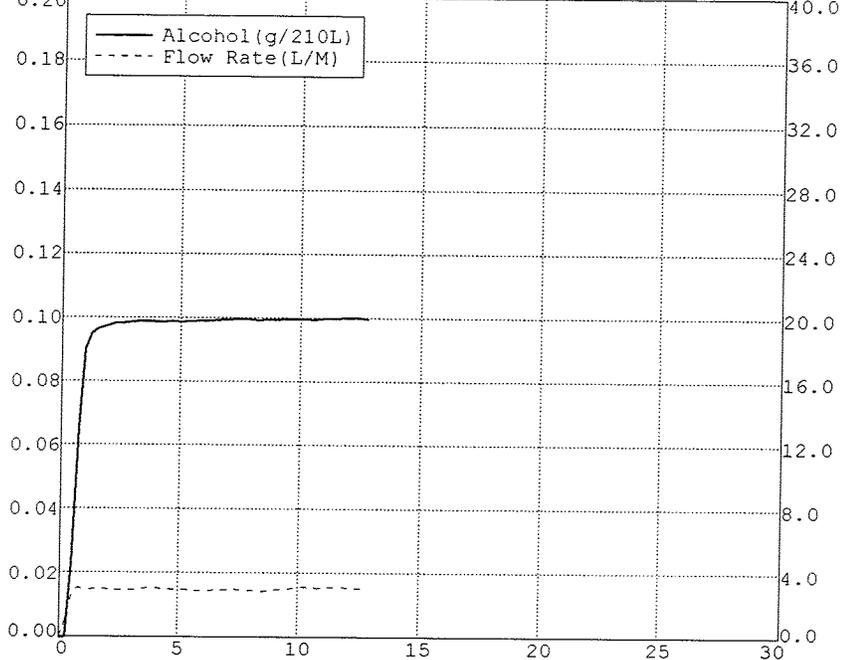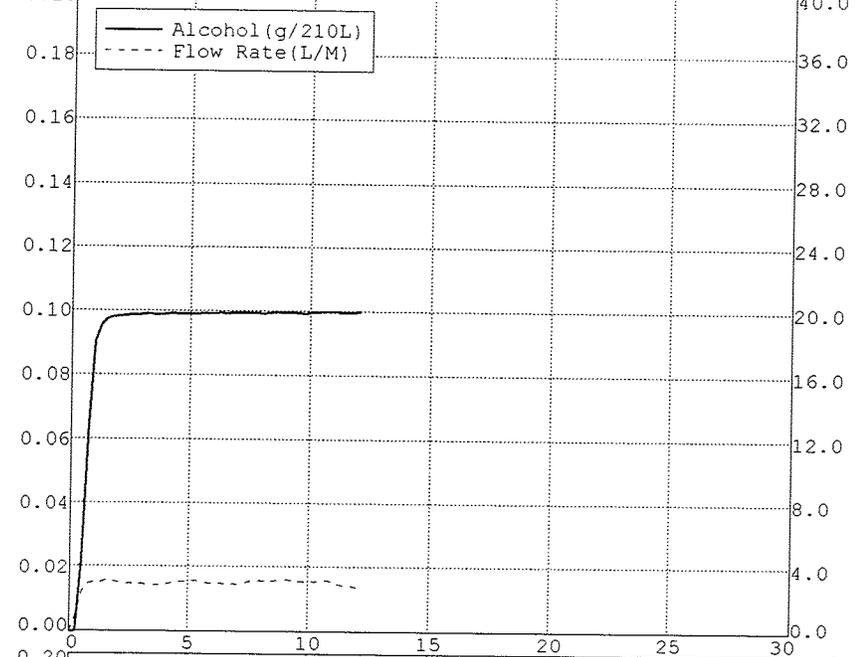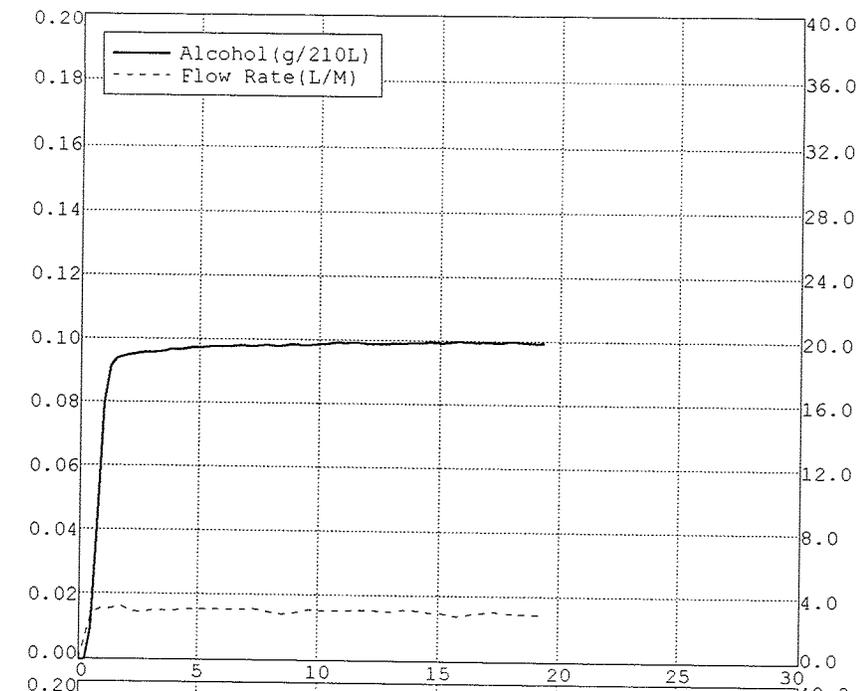

*C. B. Geisler* #248