

SUPERVISOR TEST



WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 11/24/2014

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14180

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:25
INTERNAL STANDARD	VERIFIED	07:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:25
BLANK TEST	0.00	07:26
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	07:26
BLANK TEST	0.00	07:27
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	07:27
BLANK TEST	0.00	07:28

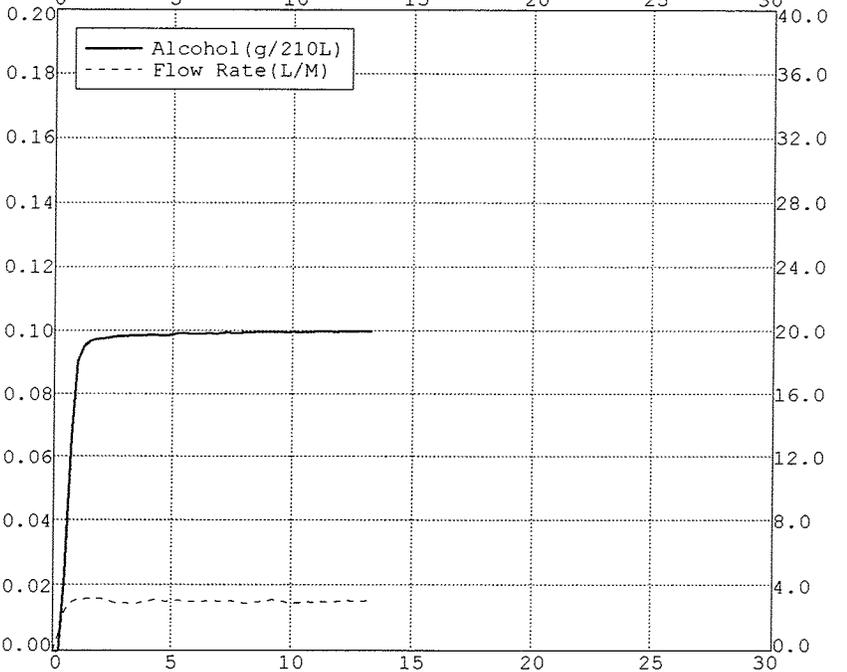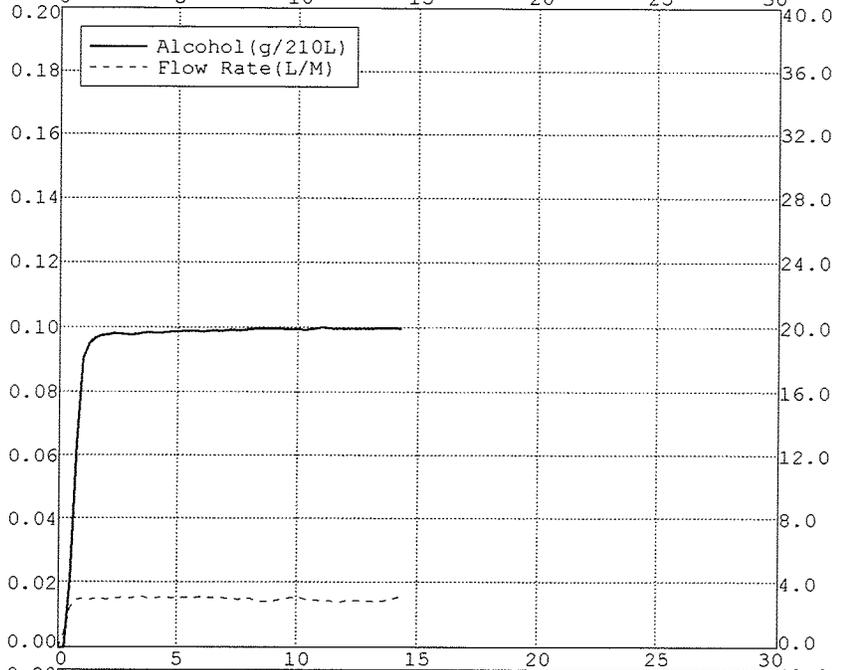

Charles B. Geisler