

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 05/19/2014

Operator Name: RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14040

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:02
INTERNAL STANDARD	VERIFIED	22:02
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	22:02
BLANK TEST	0.00	22:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:03
BLANK TEST	0.00	22:04
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	22:05
BLANK TEST	0.00	22:05

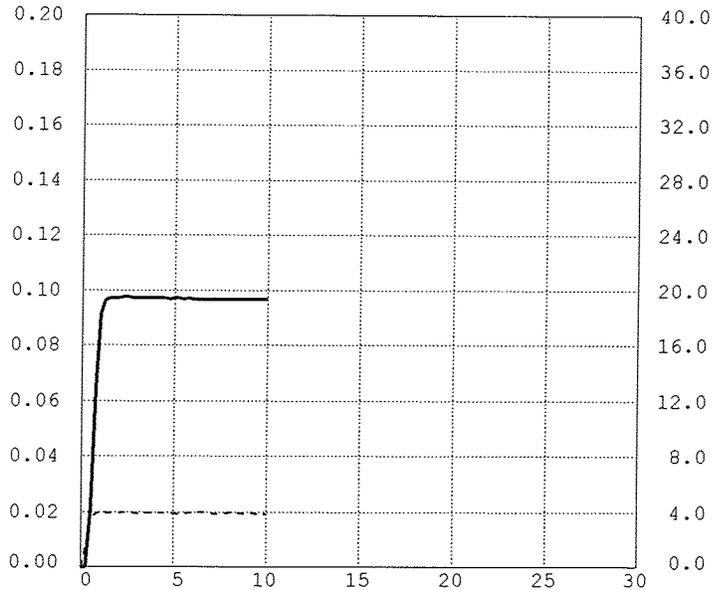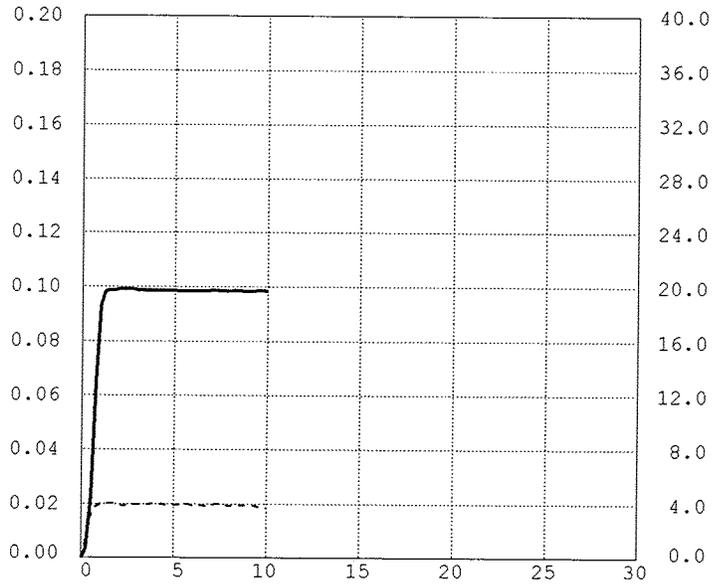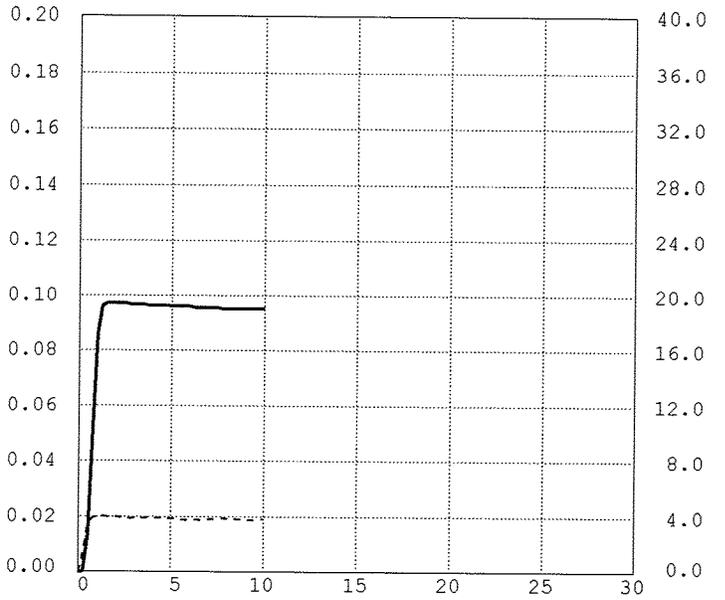

see Rpt by Bartlett case # 167 05-19-14