

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 07/21/2014

Operator Name: CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 14080

Nominal = 0.10 g/210L

|                         |          |       |
|-------------------------|----------|-------|
| BLANK TEST              | 0.00     | 14:08 |
| INTERNAL STANDARD       | VERIFIED | 14:08 |
| REFERENCE STANDARD TEMP | 34.00c   |       |
| REFERENCE STANDARD      | 0.09     | 14:08 |
| BLANK TEST              | 0.00     | 14:09 |
| REFERENCE STANDARD TEMP | 33.99c   |       |
| REFERENCE STANDARD      | 0.09     | 14:09 |
| BLANK TEST              | 0.00     | 14:10 |
| REFERENCE STANDARD TEMP | 33.99c   |       |
| REFERENCE STANDARD      | 0.09     | 14:10 |
| BLANK TEST              | 0.00     | 14:11 |

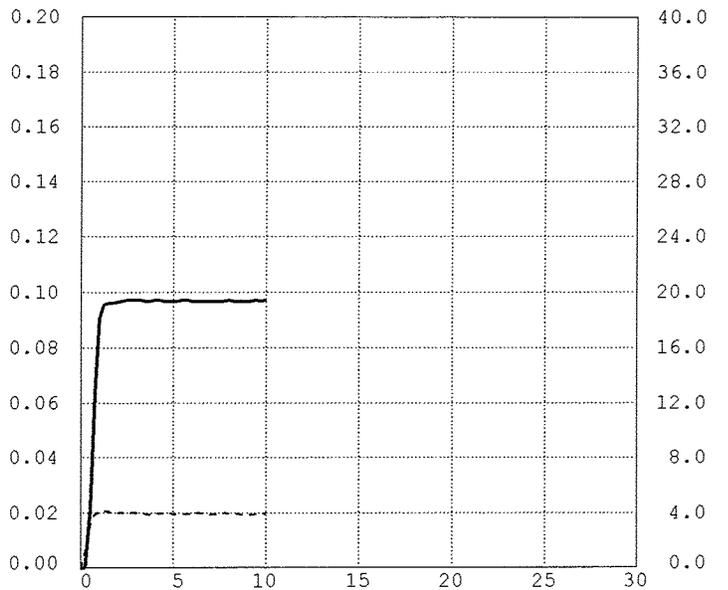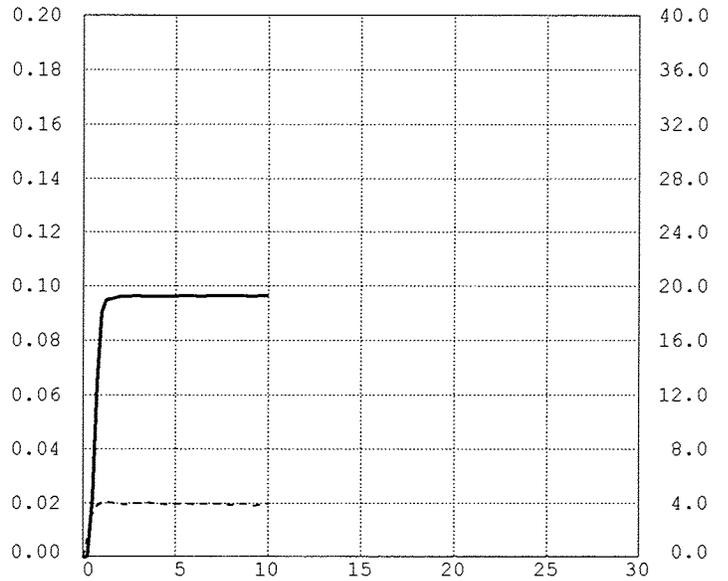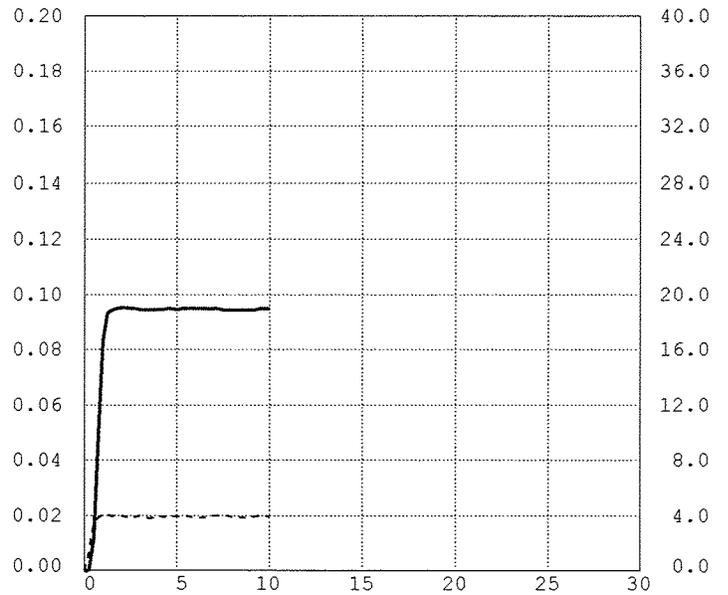

*Charles B. Geisler*  
#248  
7/21/14 1411