

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 11/10/2014

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14180

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:08
INTERNAL STANDARD	VERIFIED	17:08
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	17:08
BLANK TEST	0.00	17:09
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	17:09
BLANK TEST	0.00	17:10
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	17:10
BLANK TEST	0.00	17:11

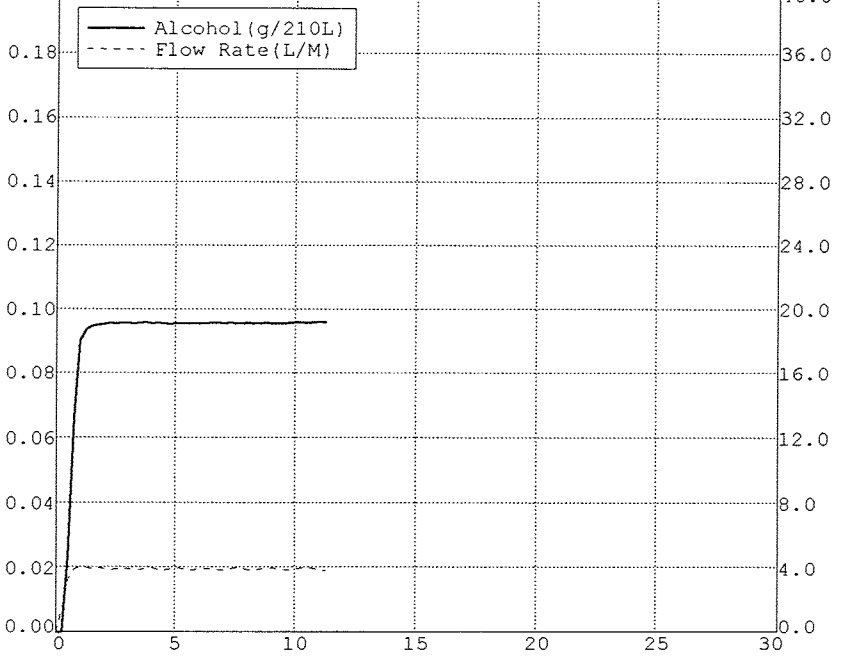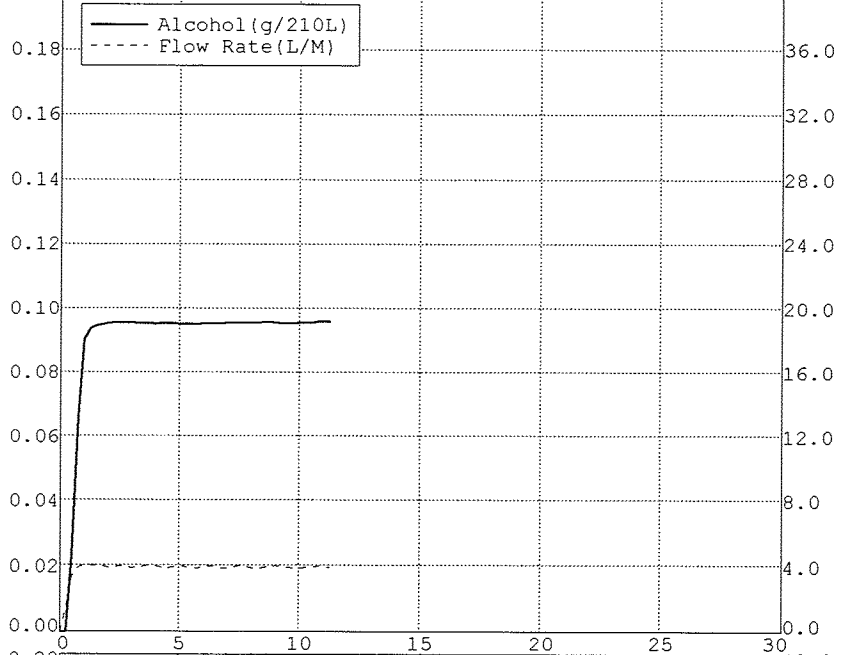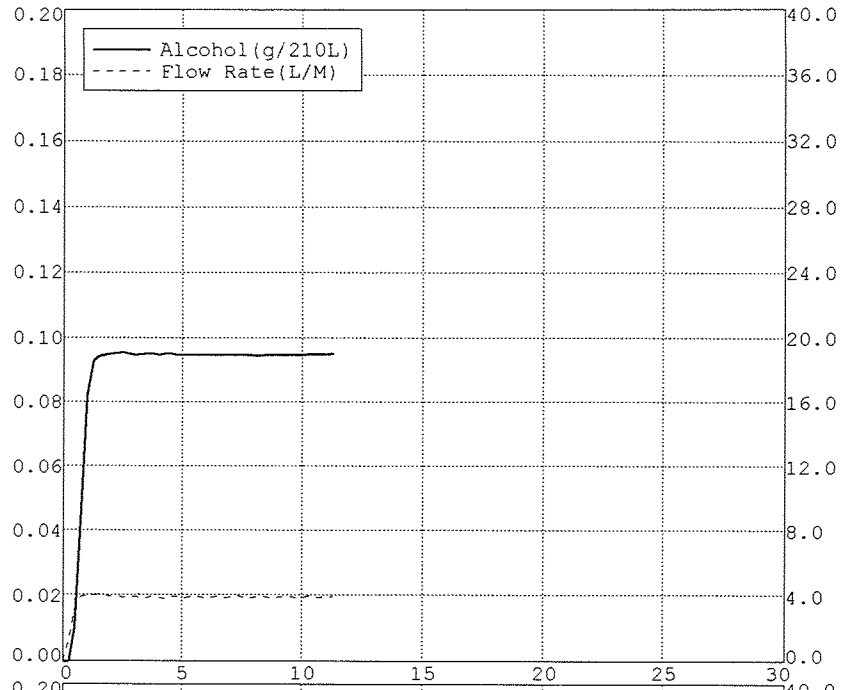

Handwritten signature: C. B. Geisler