

SUPERVISOR TEST




WARREN COUNTY
 SHERRIF'S OFFICE
 DATAMASTER dmt: 144506

Date: 12/08/2014

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 14230

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:38
INTERNAL STANDARD	VERIFIED	00:38
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:39
BLANK TEST	0.00	00:40
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:40
BLANK TEST	0.00	00:41
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:41
BLANK TEST	0.00	00:42

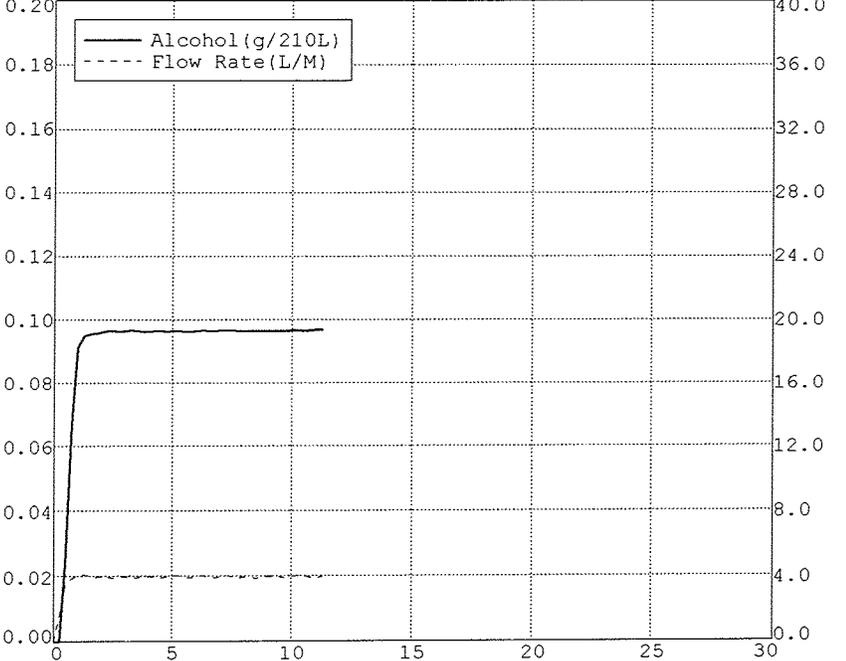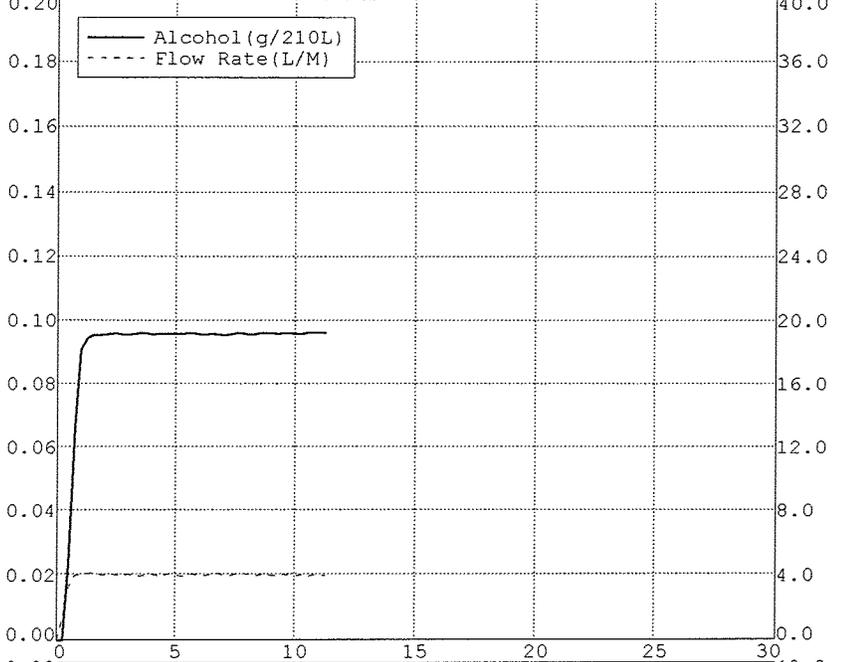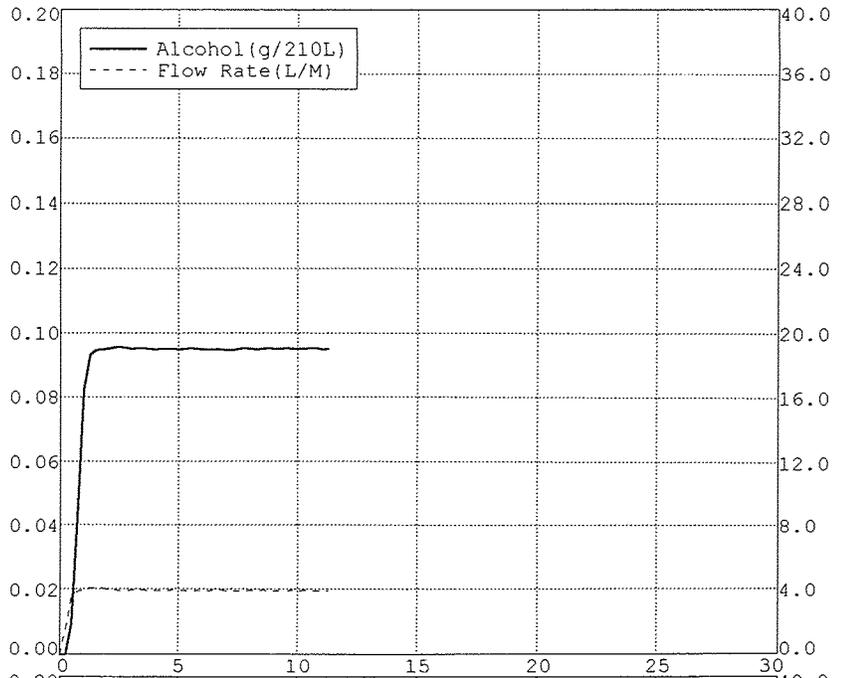

SUS Ralph J Bartlett WESO #162
 12-08-14