

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 01/19/2015

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 14230

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:12
INTERNAL STANDARD	VERIFIED	00:12
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	00:13
BLANK TEST	0.00	00:14
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:14
BLANK TEST	0.00	00:15
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:15
BLANK TEST	0.00	00:16

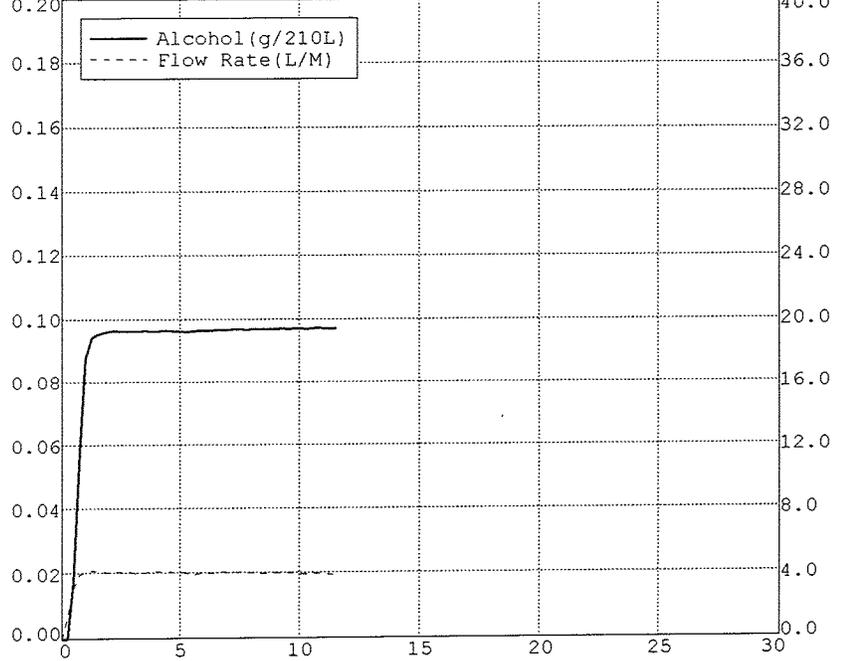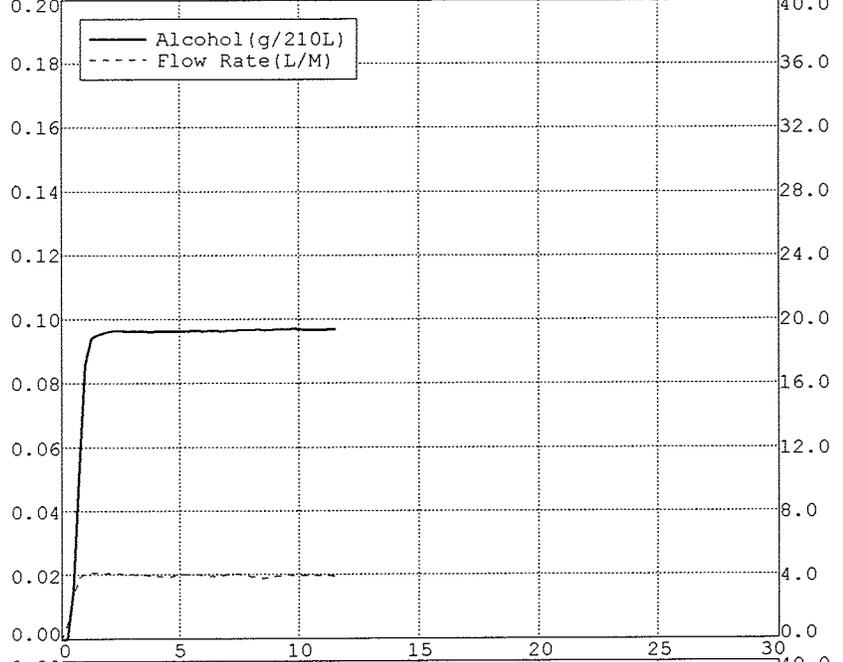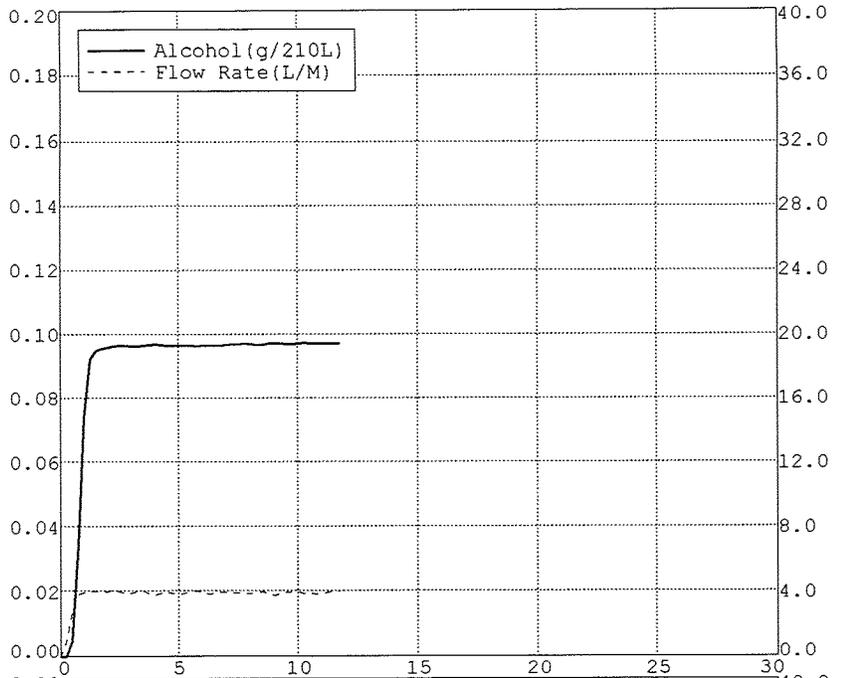

SLS RJA / Bartlett S17660 @ 10 L
 01-19-15