

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 01/27/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14230

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:45
INTERNAL STANDARD	VERIFIED	01:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:45
BLANK TEST	0.00	01:46
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	01:46
BLANK TEST	0.00	01:47
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	01:48
BLANK TEST	0.00	01:49

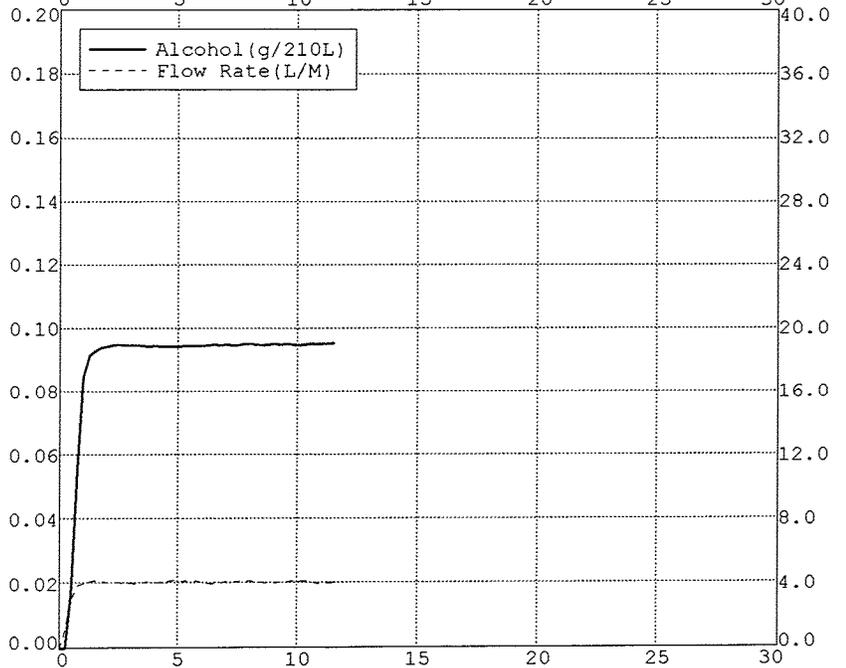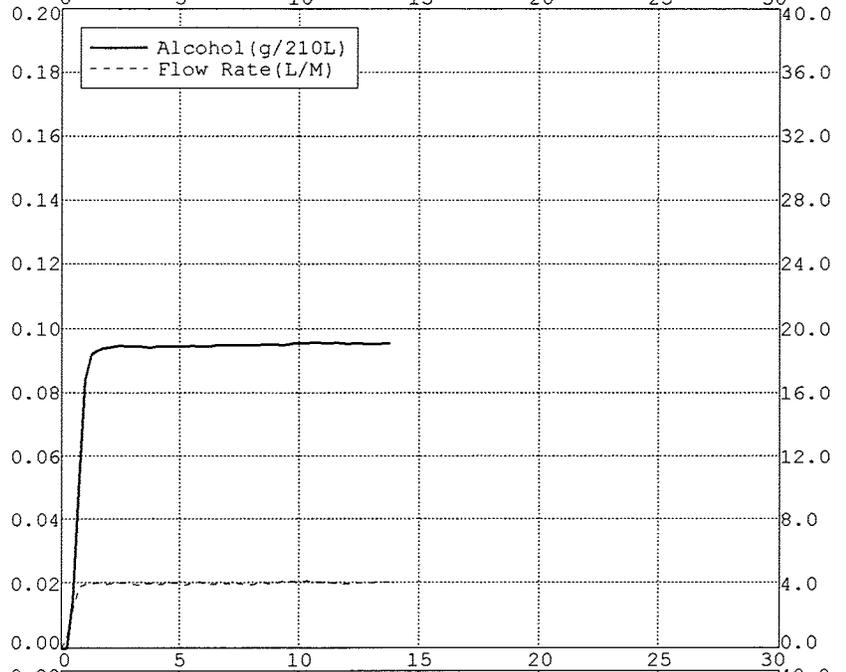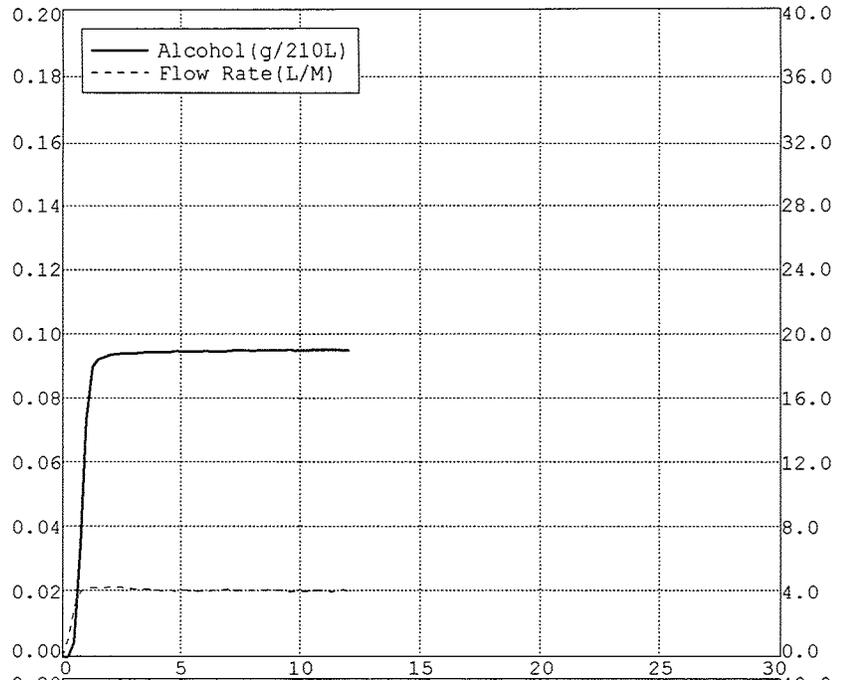

See Ralph Bartlett w/su #142
01-27-15