

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 02/16/2015

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 14260

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:49
INTERNAL STANDARD	VERIFIED	00:49
REFERENCE STANDARD TEMP	33.95c	
REFERENCE STANDARD	0.09	00:49
BLANK TEST	0.00	00:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:50
BLANK TEST	0.00	00:51
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:52
BLANK TEST	0.00	00:53

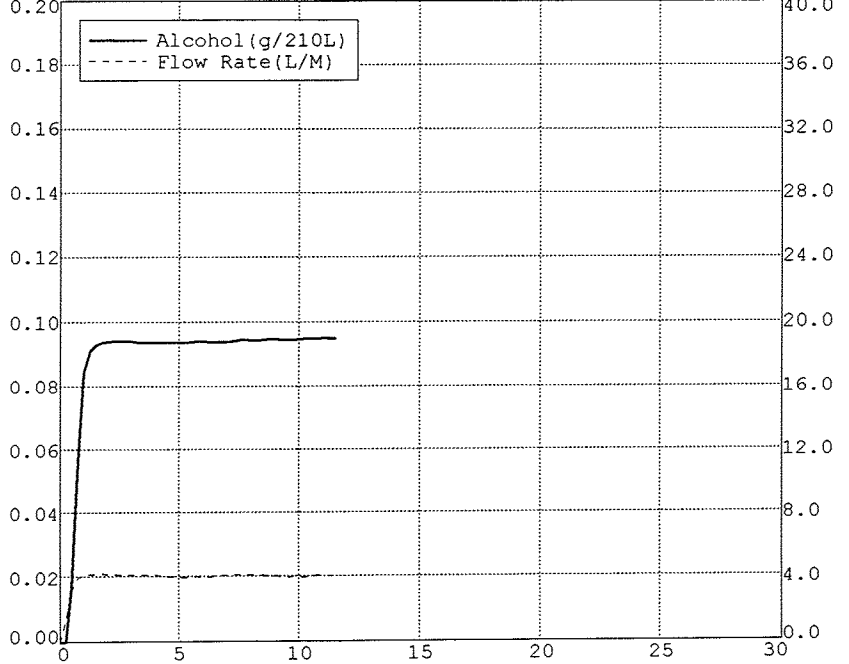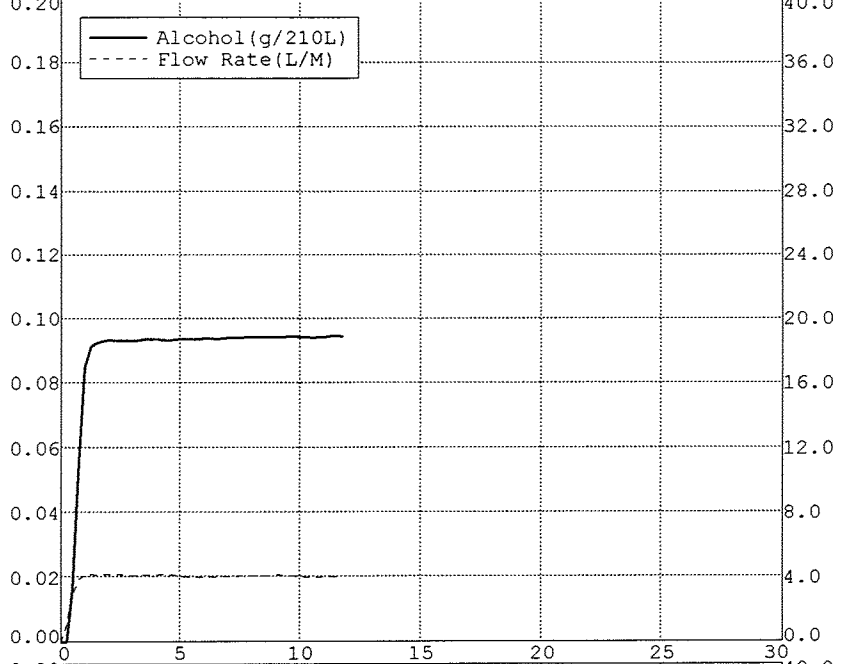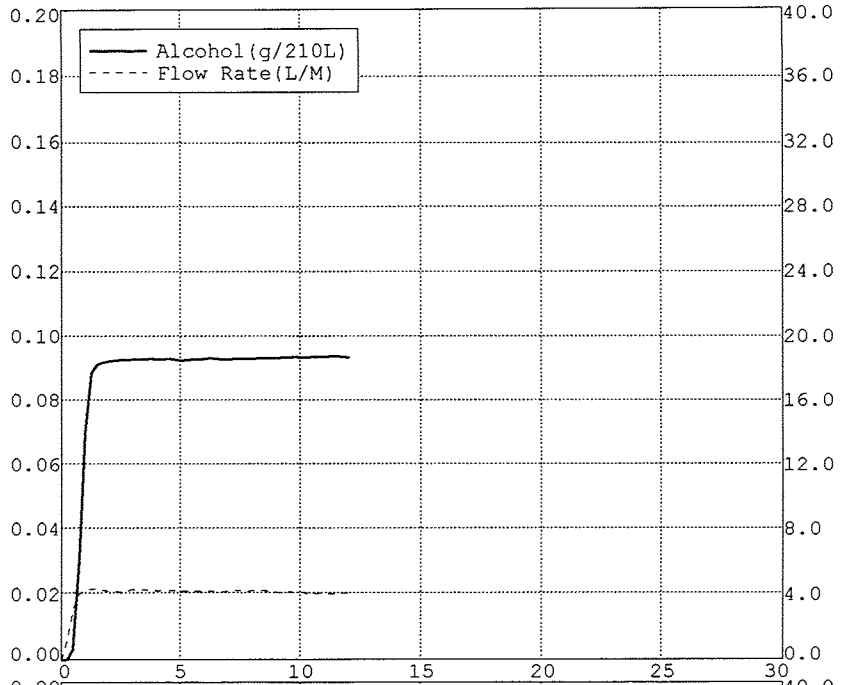

SGS RJB/B... W050 #162  
02-16-15