

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 03/16/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14260

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:38
INTERNAL STANDARD	VERIFIED	00:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:39
BLANK TEST	0.00	00:40
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:40
BLANK TEST	0.00	00:41
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:41
BLANK TEST	0.00	00:42

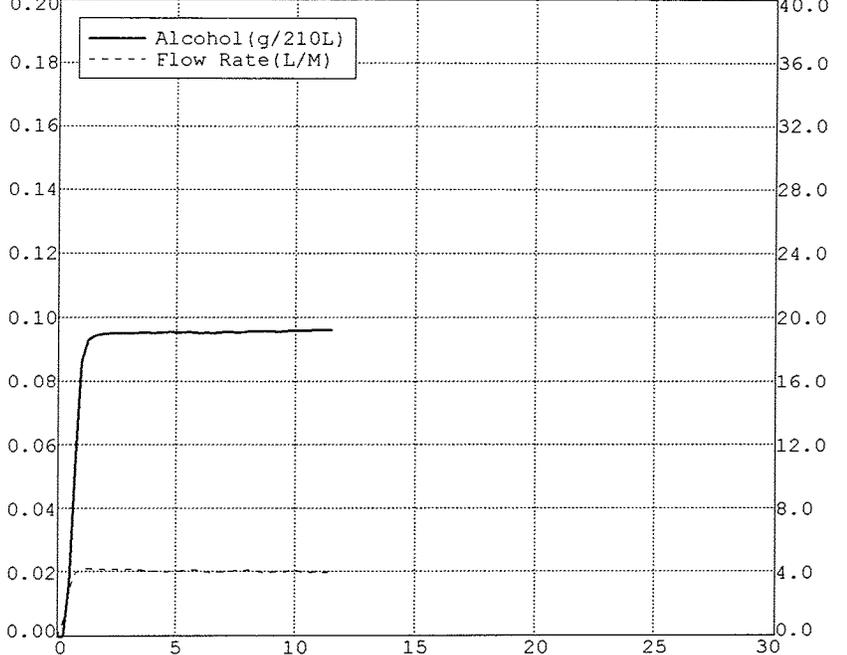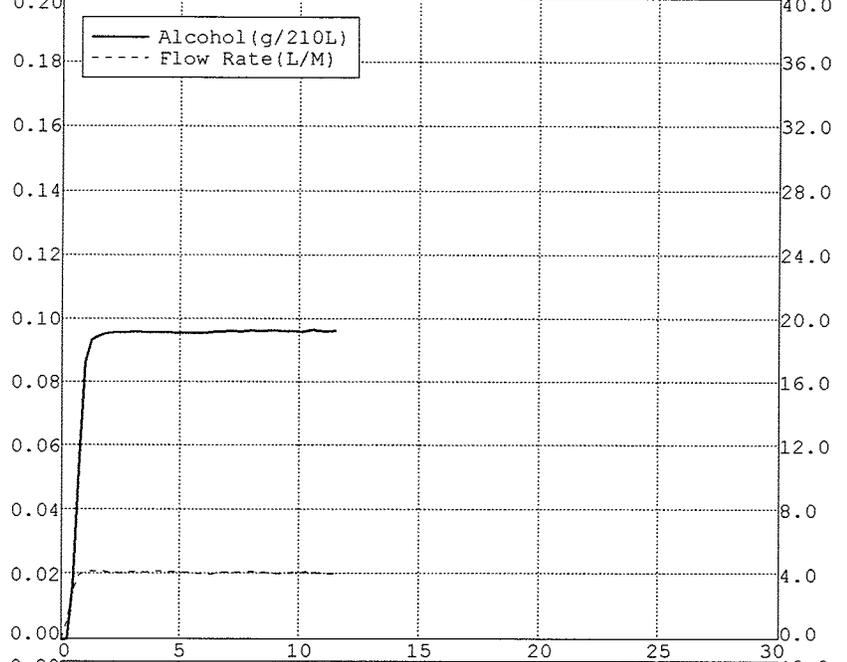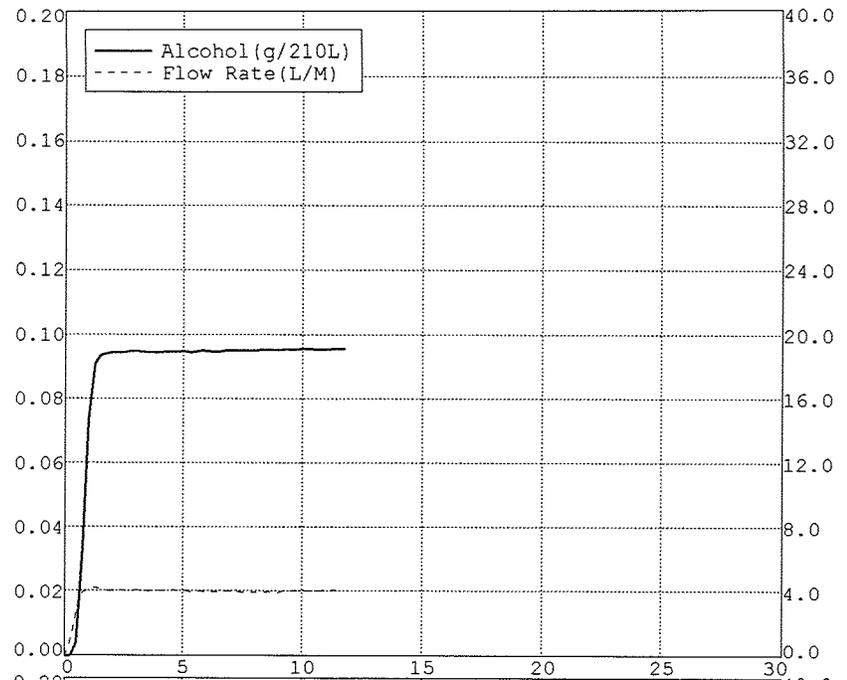

565 BT of Bartlett w/so # 162
03-16-15