

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 03/30/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15010

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:35
INTERNAL STANDARD	VERIFIED	01:35
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	01:36
BLANK TEST	0.00	01:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:37
BLANK TEST	0.00	01:38
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	01:39
BLANK TEST	0.00	01:40

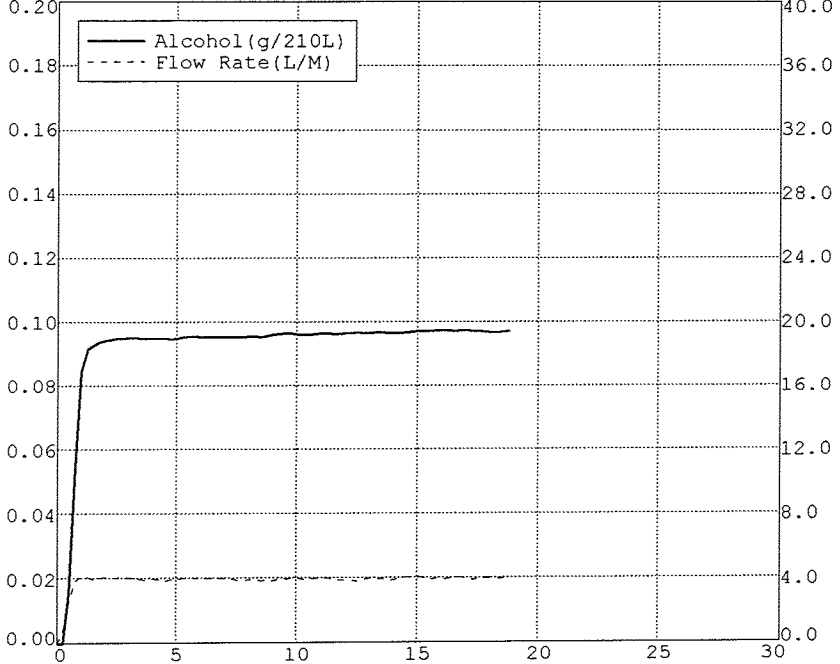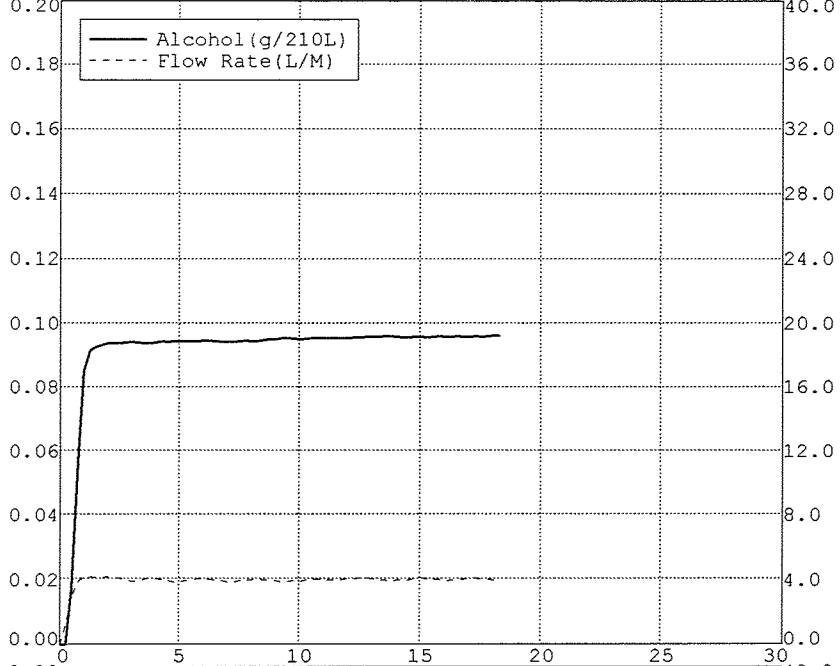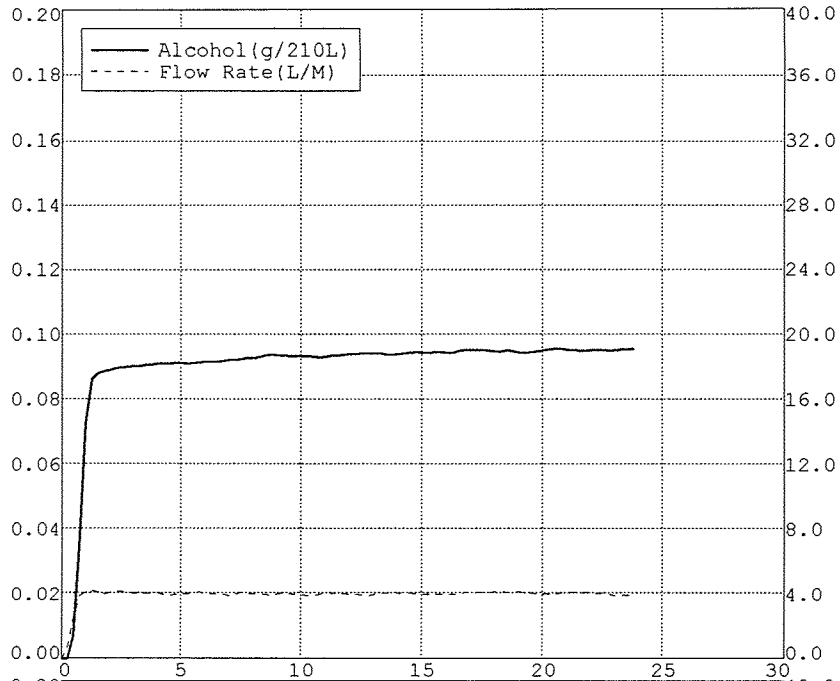

SGS *RJ Bartlett* WISO #162
03-30-15