

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 04/27/2015

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15010

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:44
INTERNAL STANDARD	VERIFIED	08:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:45
BLANK TEST	0.00	08:46
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	08:46
BLANK TEST	0.00	08:47
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	08:47
BLANK TEST	0.00	08:48

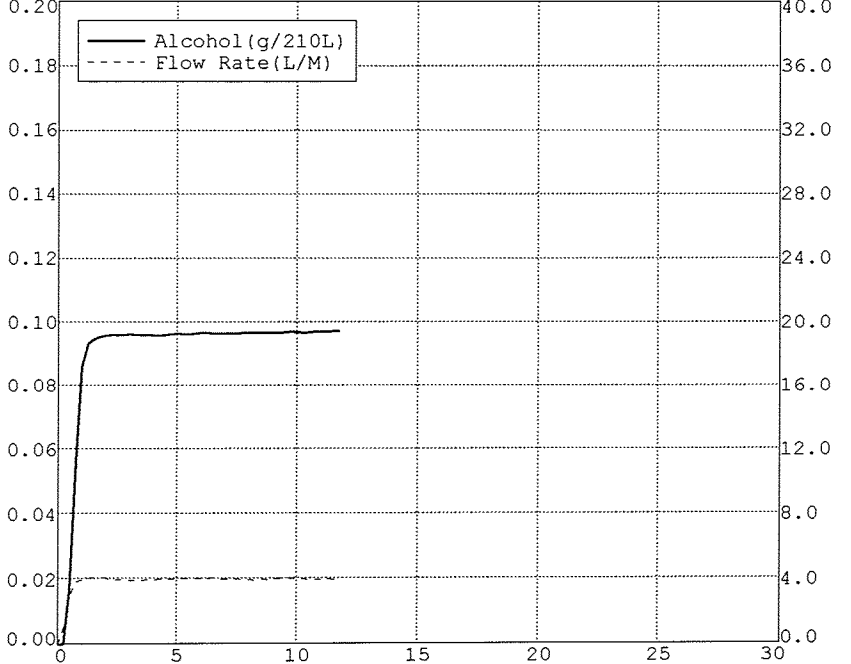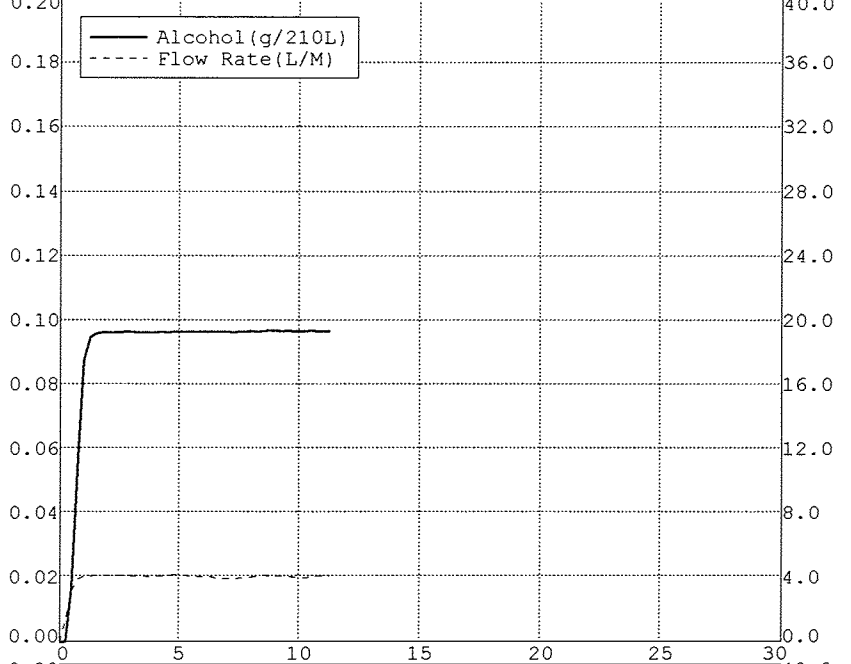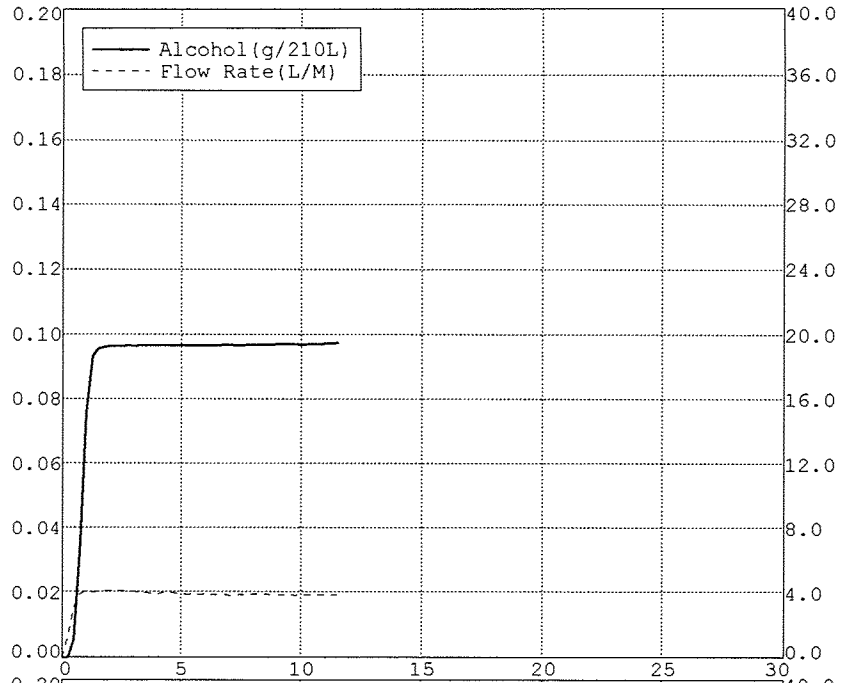

Handwritten signature: C. B. Geisler #33757