

SUPERVISOR TEST




 WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 05/25/2015

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 15010

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:49
INTERNAL STANDARD	VERIFIED	01:50
REFERENCE STANDARD TEMP	33.95c	
REFERENCE STANDARD	0.09	01:50
BLANK TEST	0.00	01:51
REFERENCE STANDARD TEMP	33.94c	
REFERENCE STANDARD	0.09	01:51
BLANK TEST	0.00	01:52
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	01:53
BLANK TEST	0.00	01:53

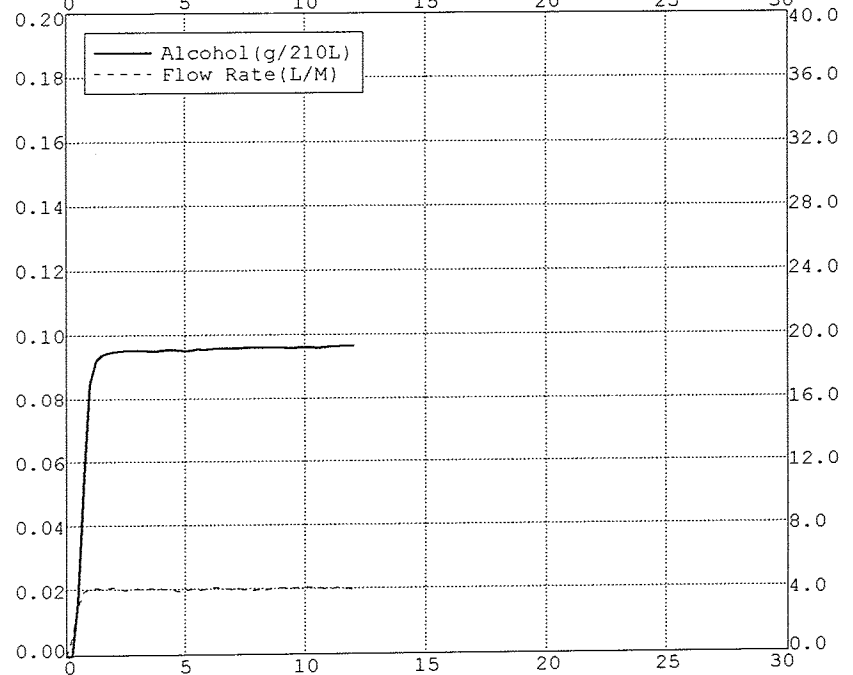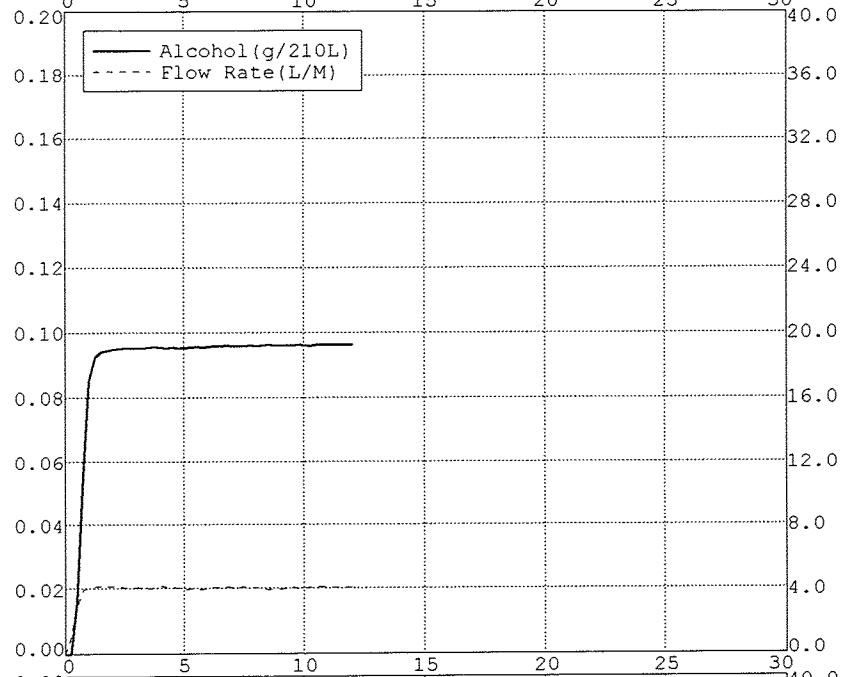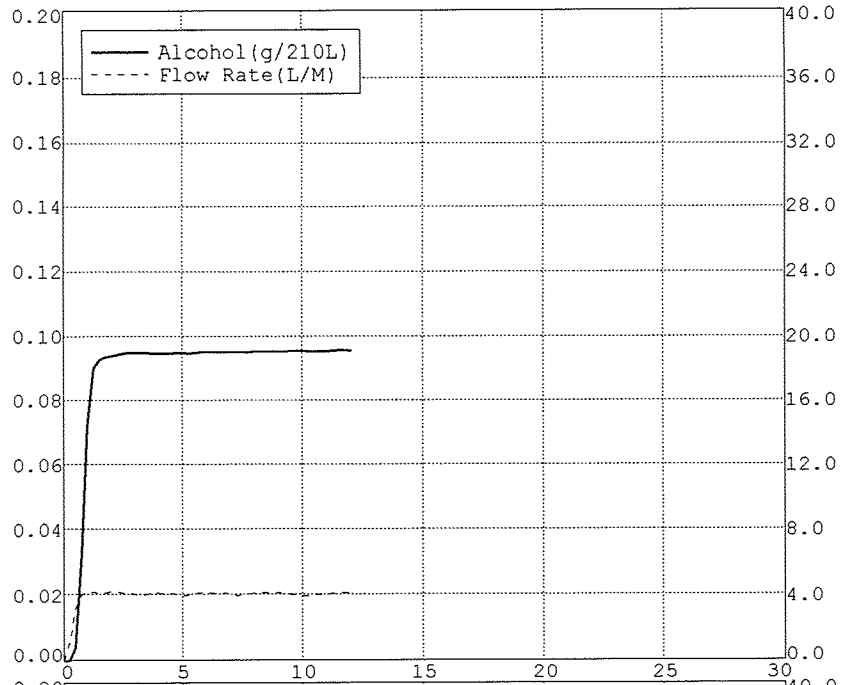

SOS *Ralph Bartlett* #162
 05-25-15