

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 06/16/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15070

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:46
INTERNAL STANDARD	VERIFIED	00:46
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.09	00:47
BLANK TEST	0.00	00:47
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:48
BLANK TEST	0.00	00:49
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	00:49
BLANK TEST	0.00	00:50

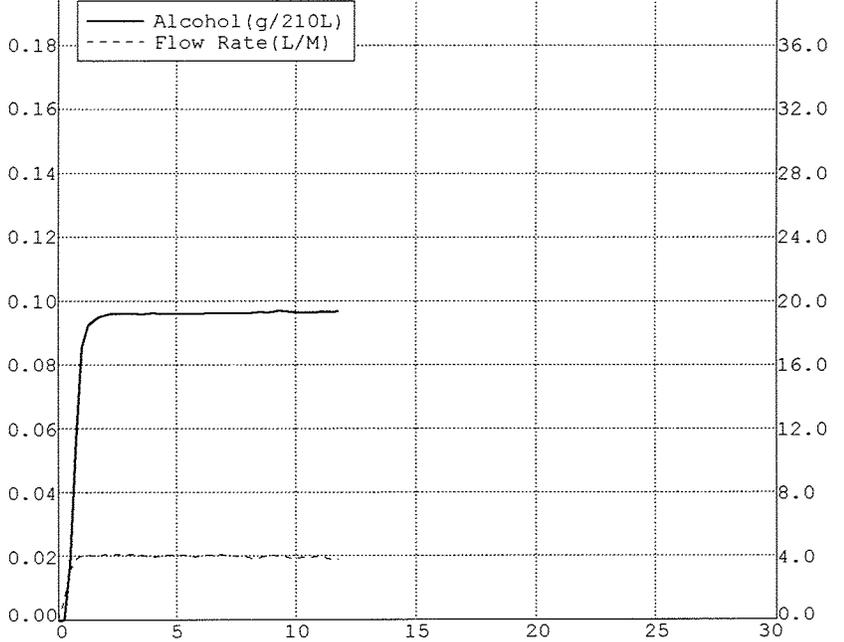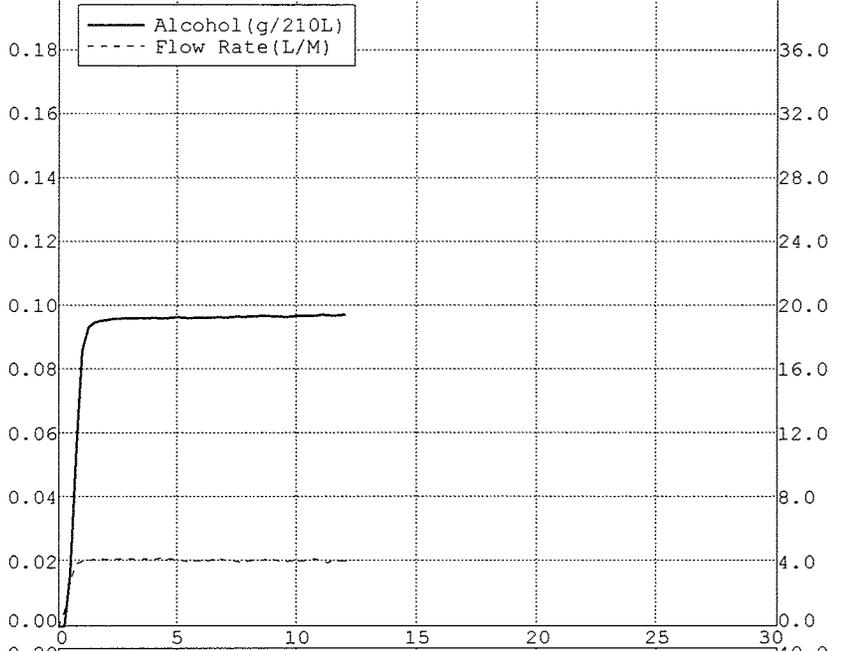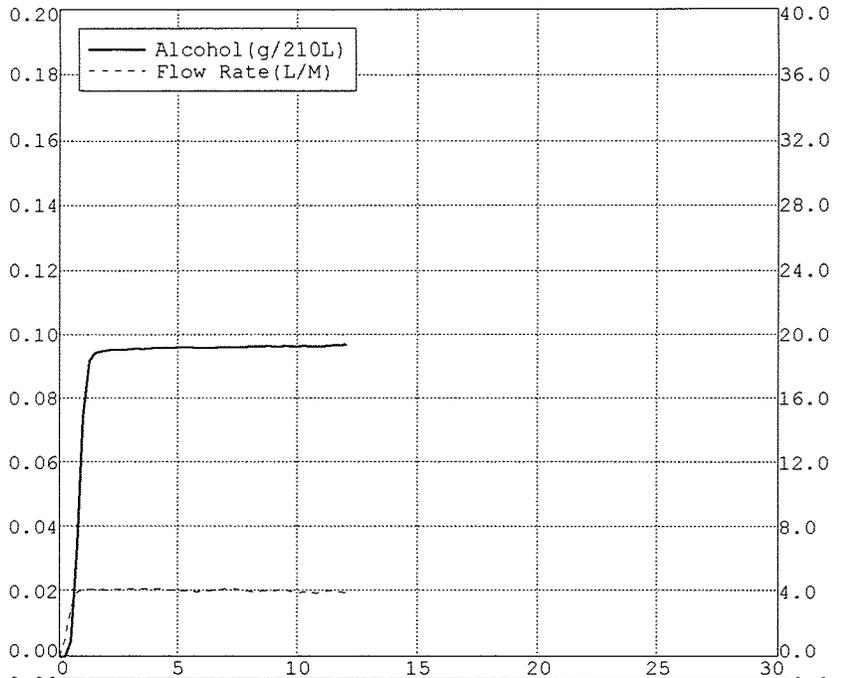

565 RJP Initial were #162
06/16/15