

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 06/22/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15070

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:03
INTERNAL STANDARD	VERIFIED	02:03
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	02:04
BLANK TEST	0.00	02:05
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	02:05
BLANK TEST	0.00	02:06
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	02:06
BLANK TEST	0.00	02:07

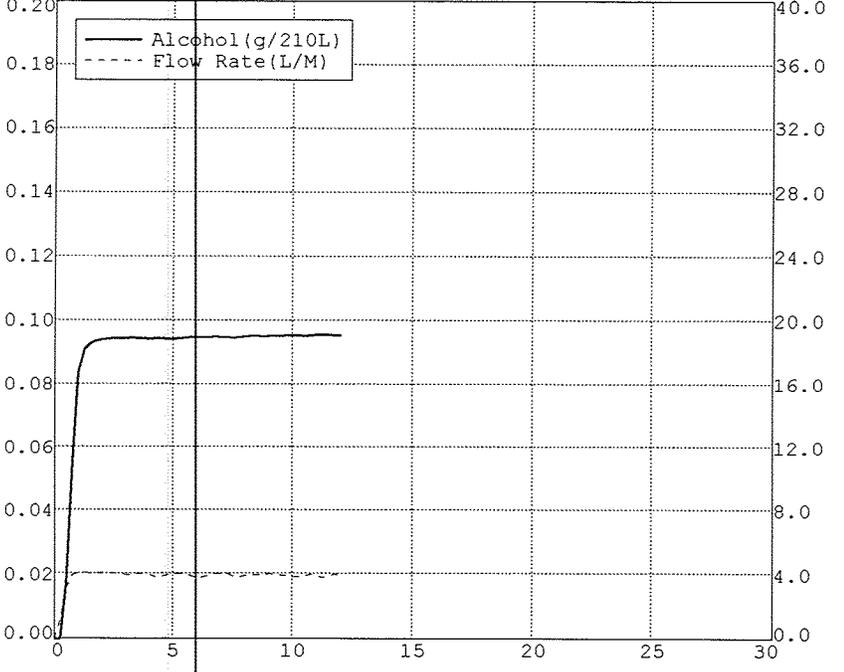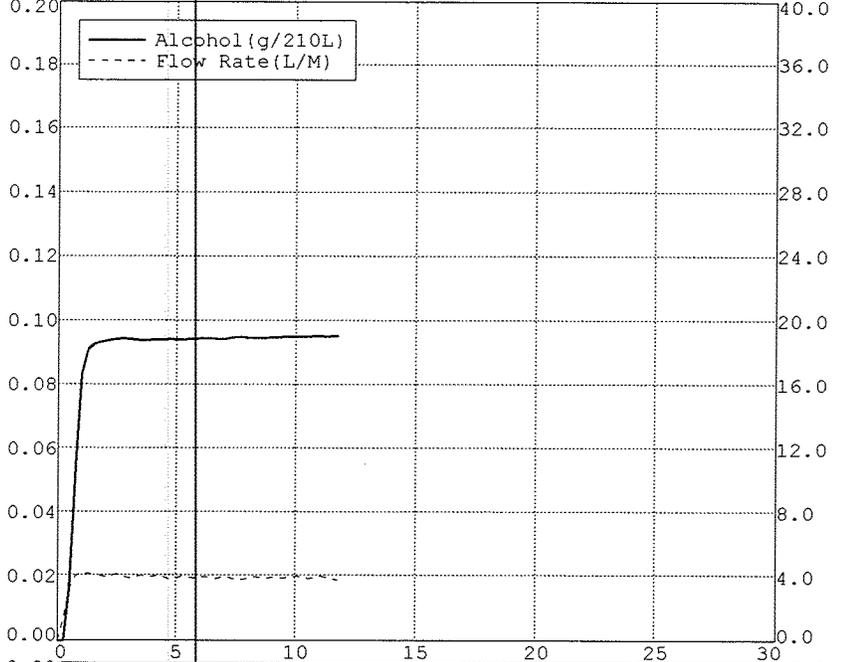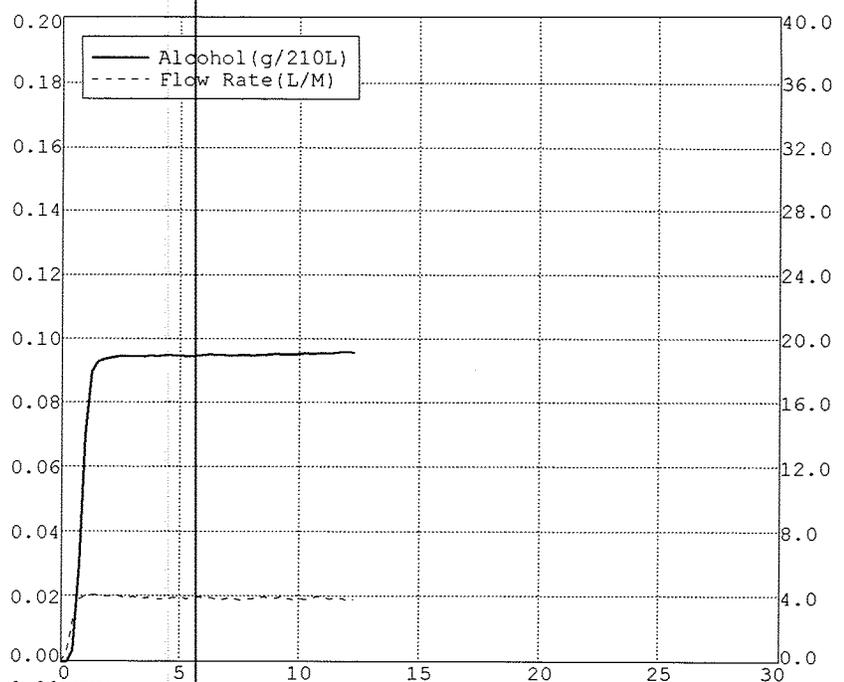

Sgt. Ralph Bartlett WESO #112
06-22-15