

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 07/06/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15070

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:58
INTERNAL STANDARD	VERIFIED	01:58
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	01:58
BLANK TEST	0.00	01:59
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	01:59
BLANK TEST	0.00	02:00
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	02:01
BLANK TEST	0.00	02:02

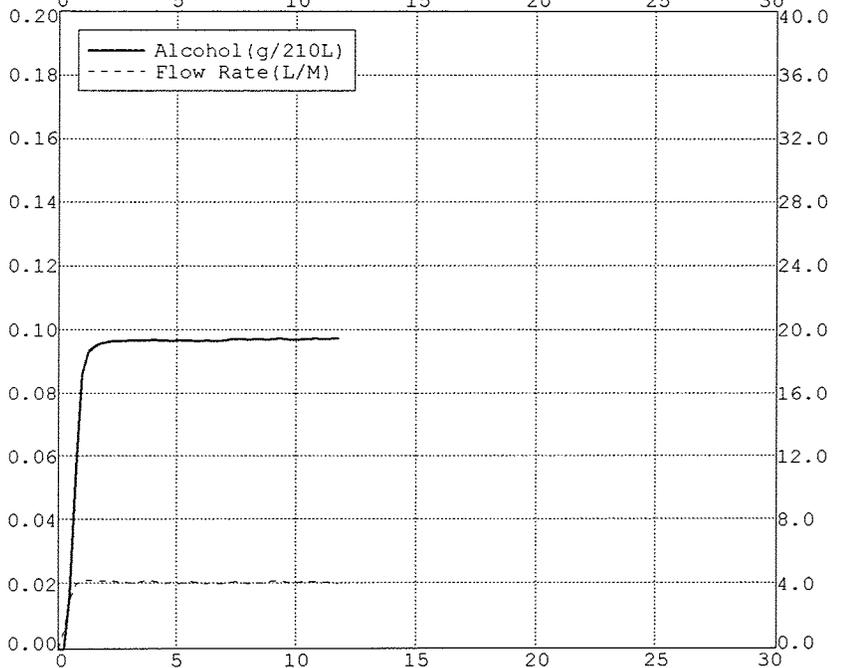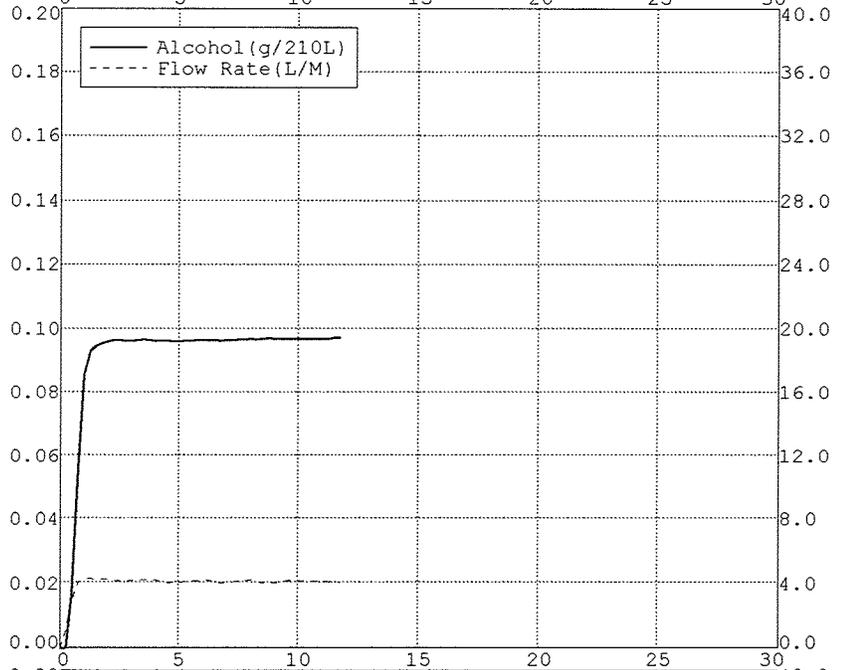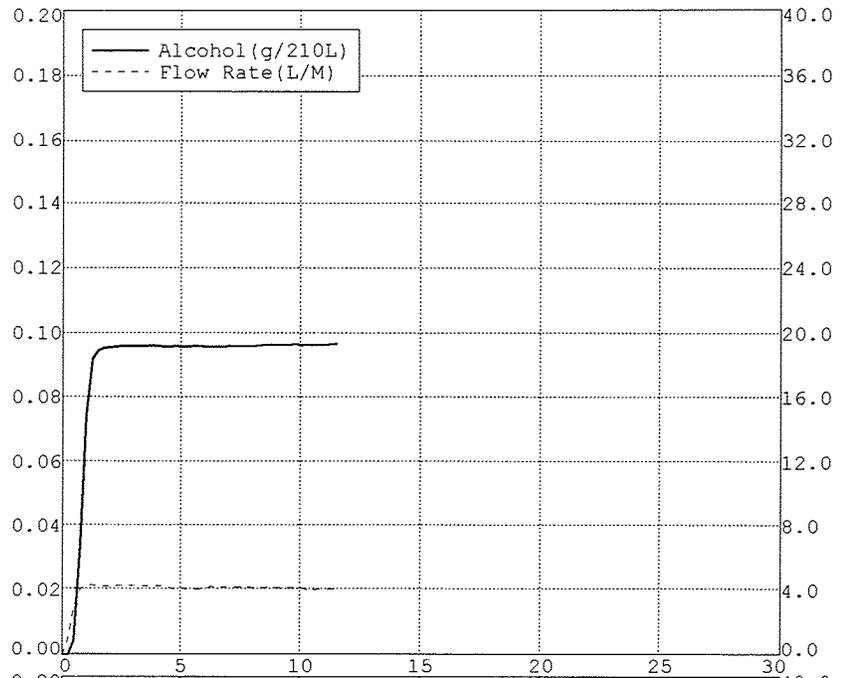

365 Ralph J Bartlett weso #162
07-06-15