

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 08/12/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15140

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:07
INTERNAL STANDARD	VERIFIED	01:08
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	01:08
BLANK TEST	0.00	01:09
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	01:09
BLANK TEST	0.00	01:10
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	01:11
BLANK TEST	0.00	01:12

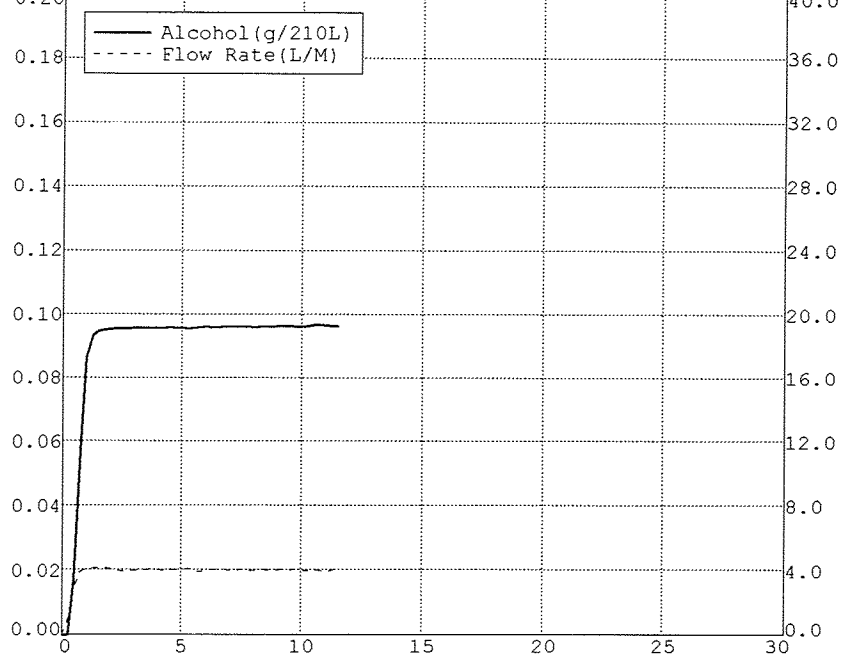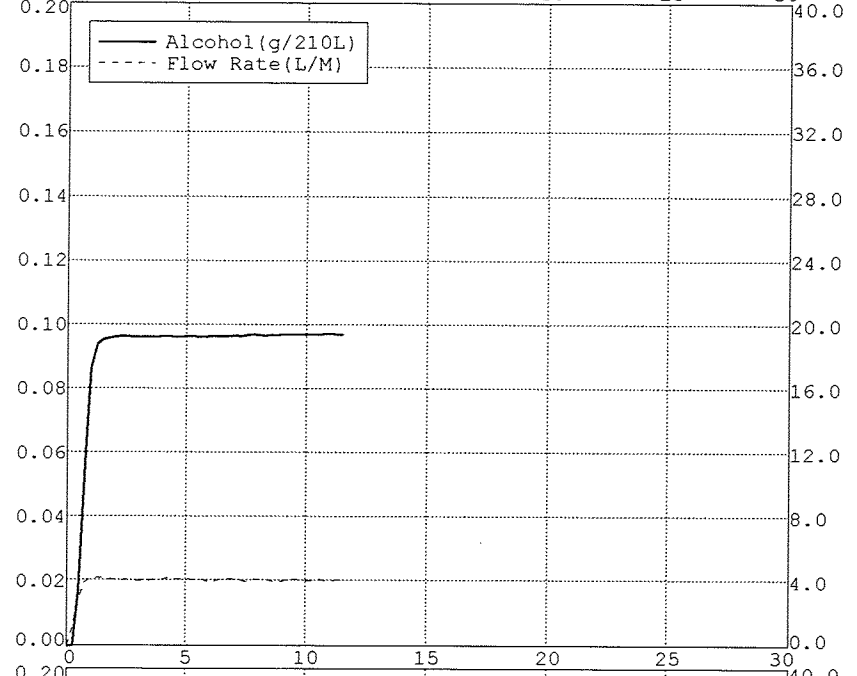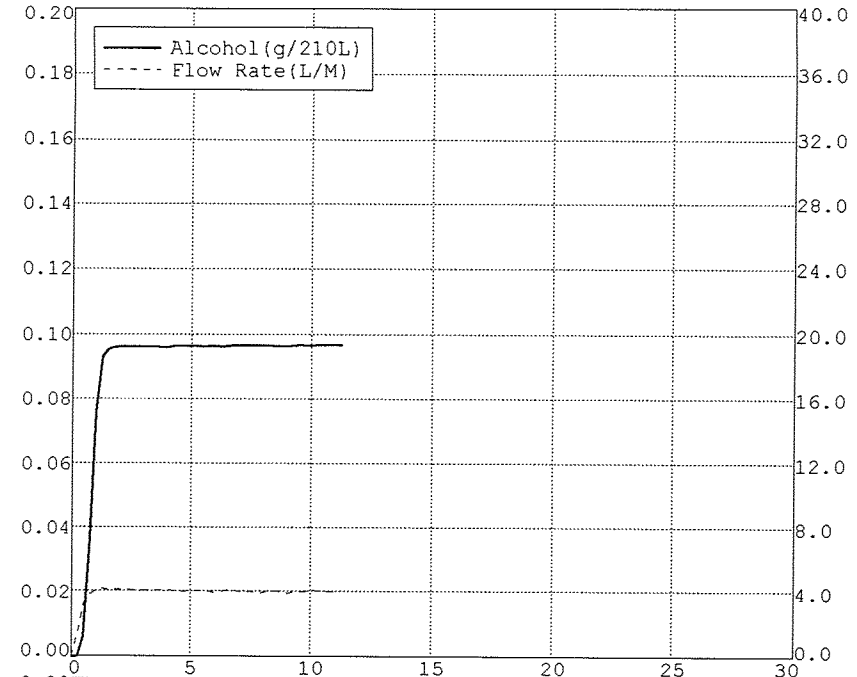

SOS *RJ Bartlett* WESO #162
08-12-15