

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 08/25/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15140

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:27
INTERNAL STANDARD	VERIFIED	02:27
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	02:28
BLANK TEST	0.00	02:29
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	02:29
BLANK TEST	0.00	02:30
REFERENCE STANDARD TEMP	33.95c	
REFERENCE STANDARD	0.09	02:30
BLANK TEST	0.00	02:31

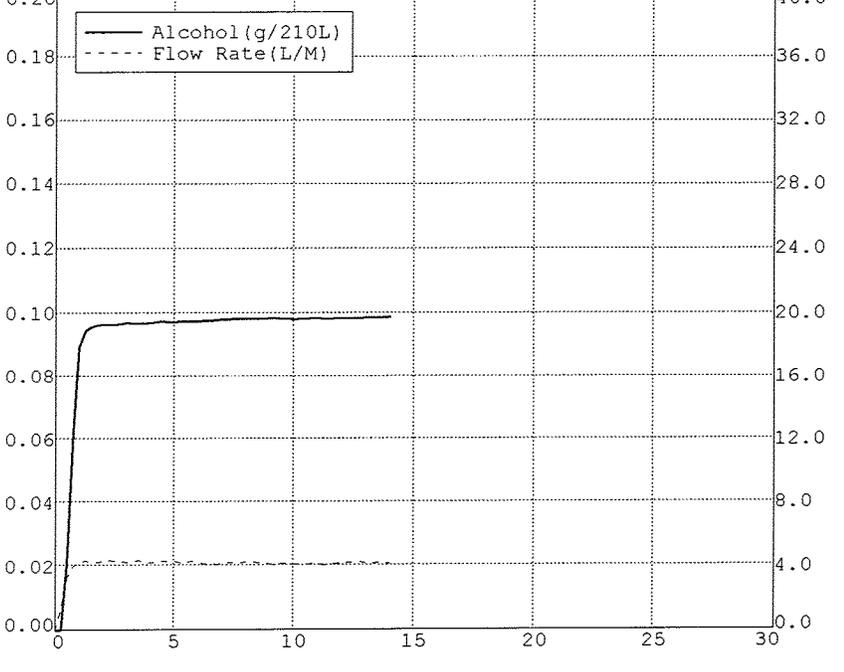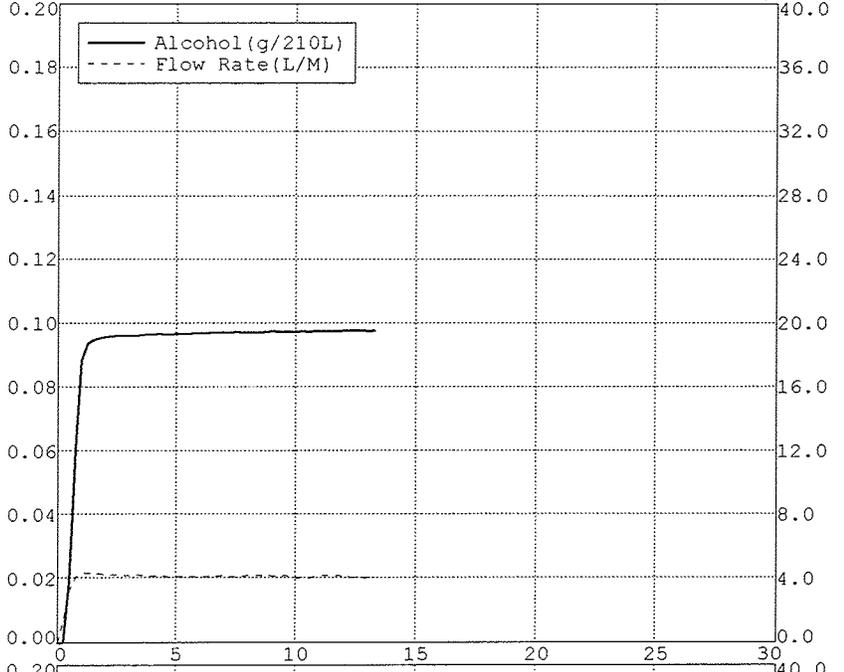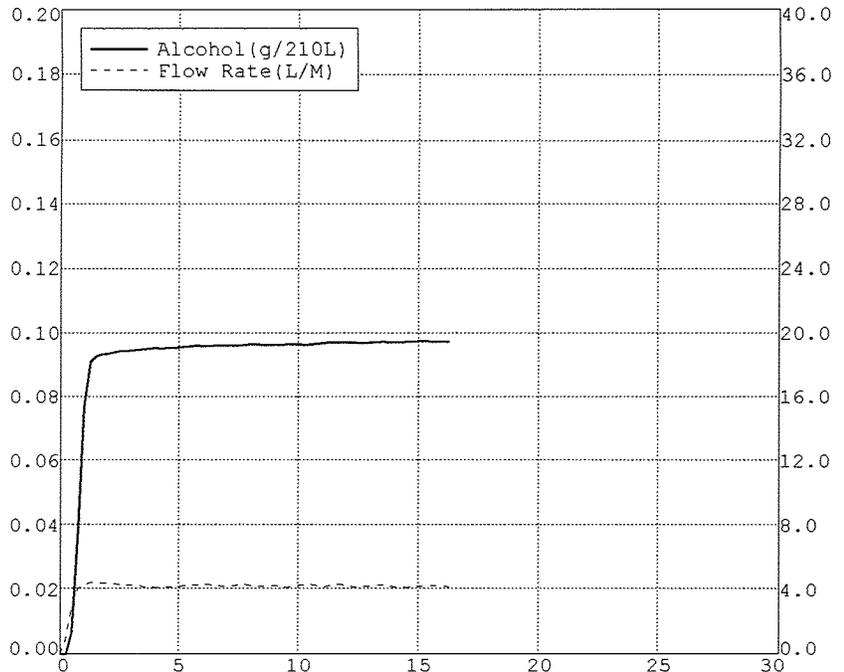

SGS RBH J. Bartlett WSO #162
08/25/15