

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 08/31/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15140

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:39
INTERNAL STANDARD	VERIFIED	00:39
REFERENCE STANDARD TEMP	33.95c	
REFERENCE STANDARD	0.09	00:39
BLANK TEST	0.00	00:40
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:41
BLANK TEST	0.00	00:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:42
BLANK TEST	0.00	00:43

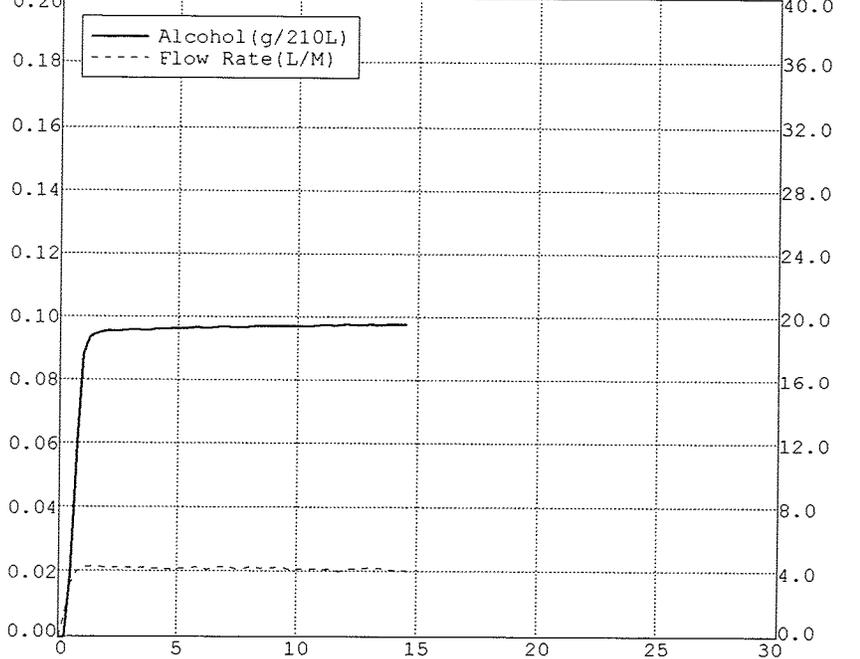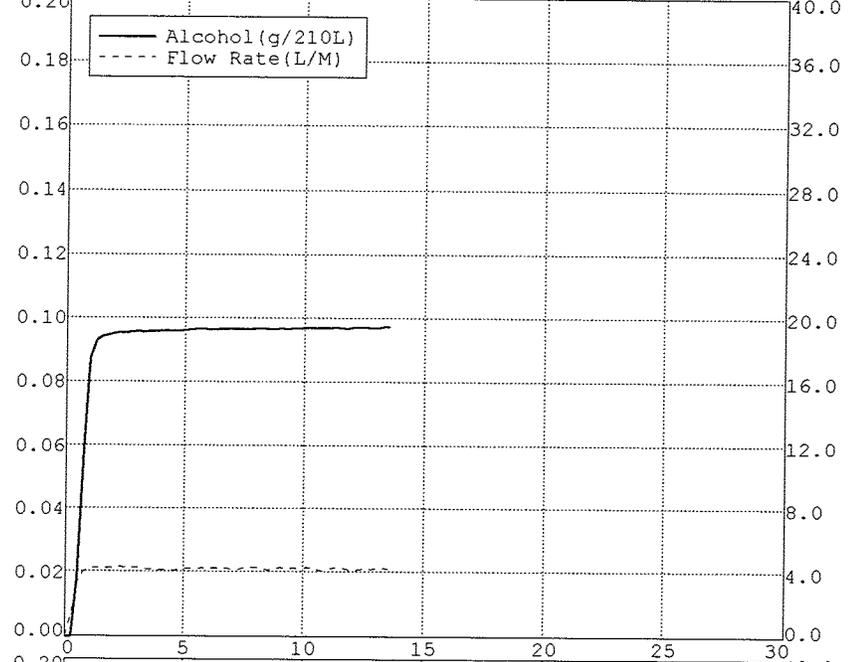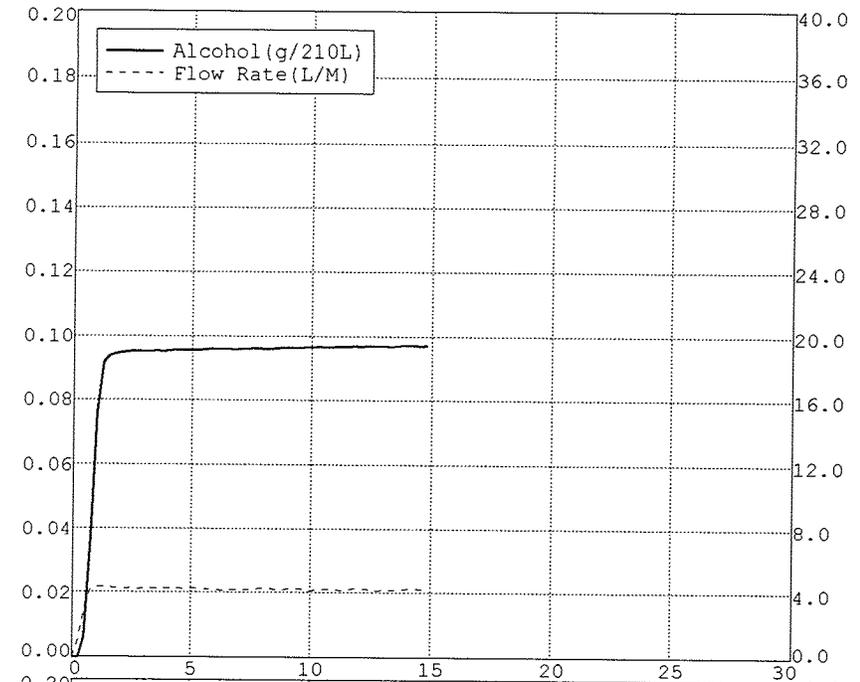

505 RLB / Bartlett WSO #162
08-31-15