

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 09/17/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15140

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:14
INTERNAL STANDARD	VERIFIED	01:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:15
BLANK TEST	0.00	01:15
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	01:16
BLANK TEST	0.00	01:17
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	01:17
BLANK TEST	0.00	01:18

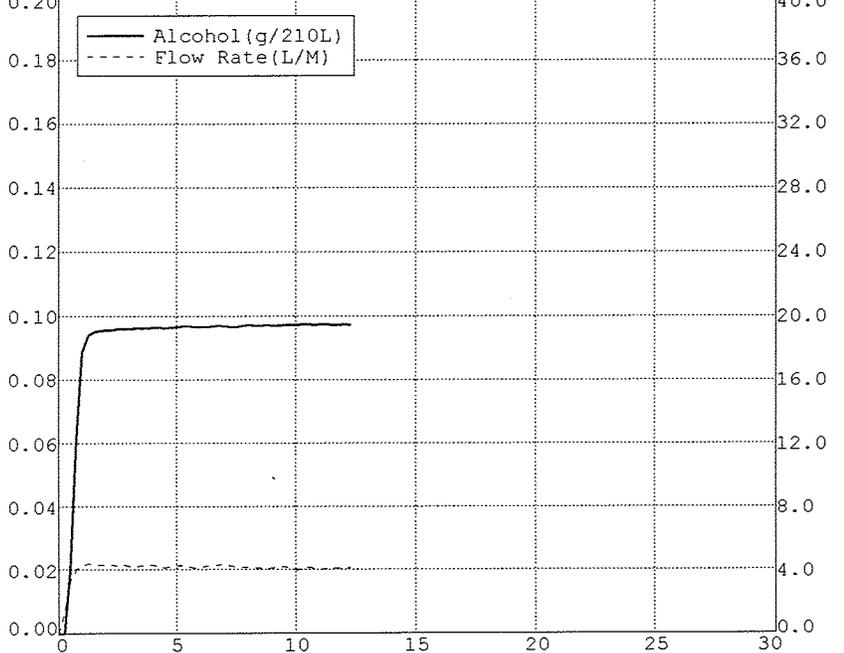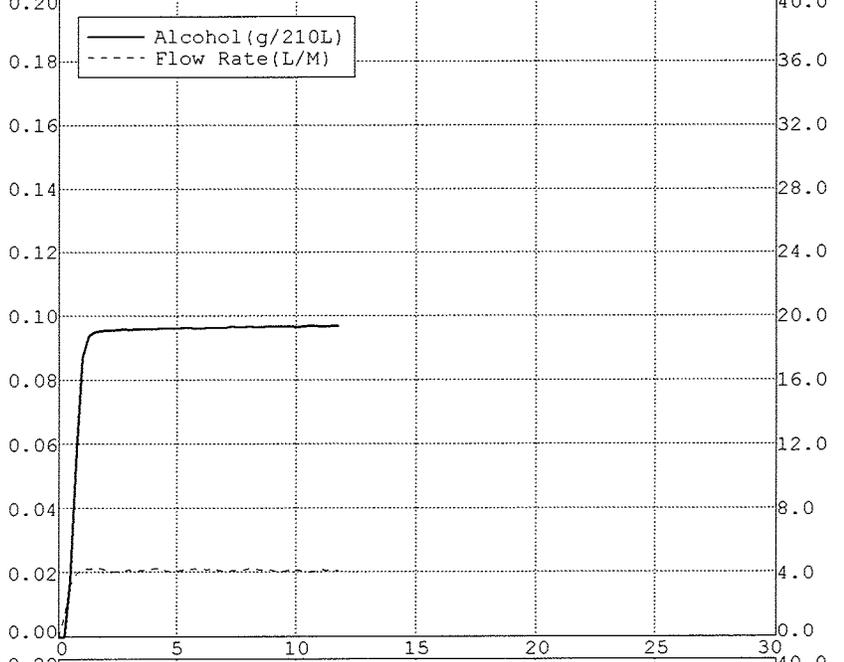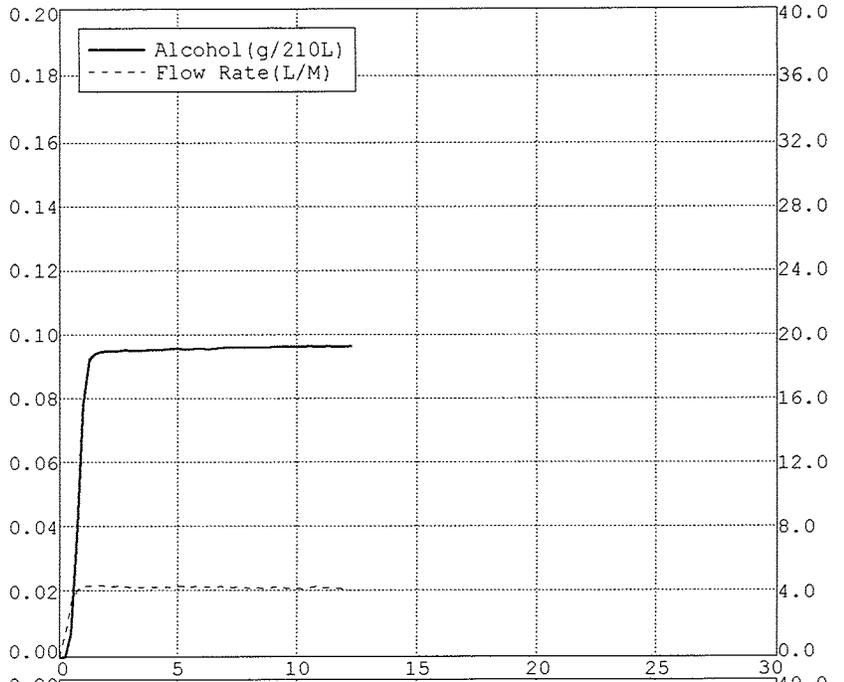

SUS BH / Bartlett WC10 #162

09-17-15