

SUPERVISOR TEST




WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 105208

Date: 09/22/2015

OPERATOR NAME:  
 RALPH J BARTLETT  
 Permit #: 26222  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 15140

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:58
INTERNAL STANDARD	VERIFIED	01:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:58
BLANK TEST	0.00	01:59
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	02:00
BLANK TEST	0.00	02:01
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:01
BLANK TEST	0.00	02:02

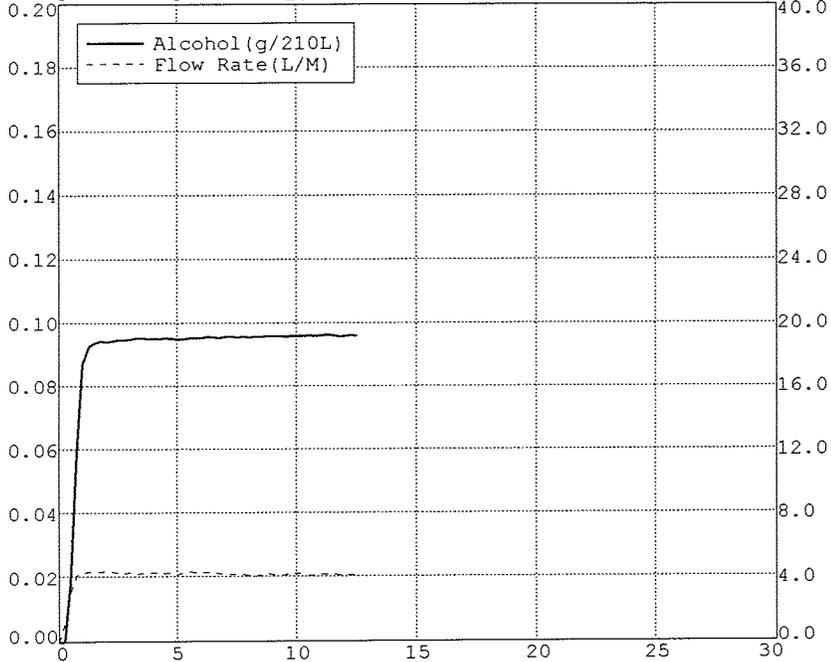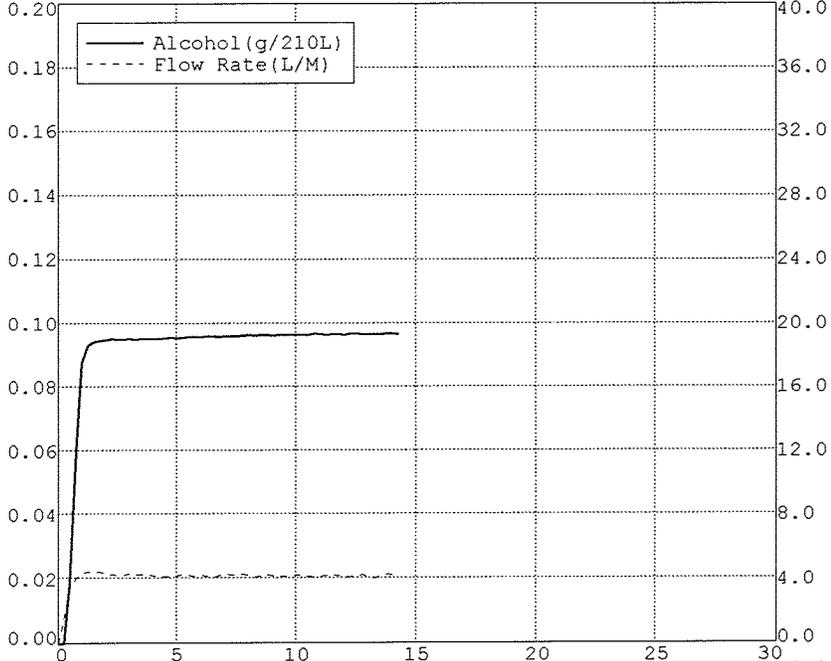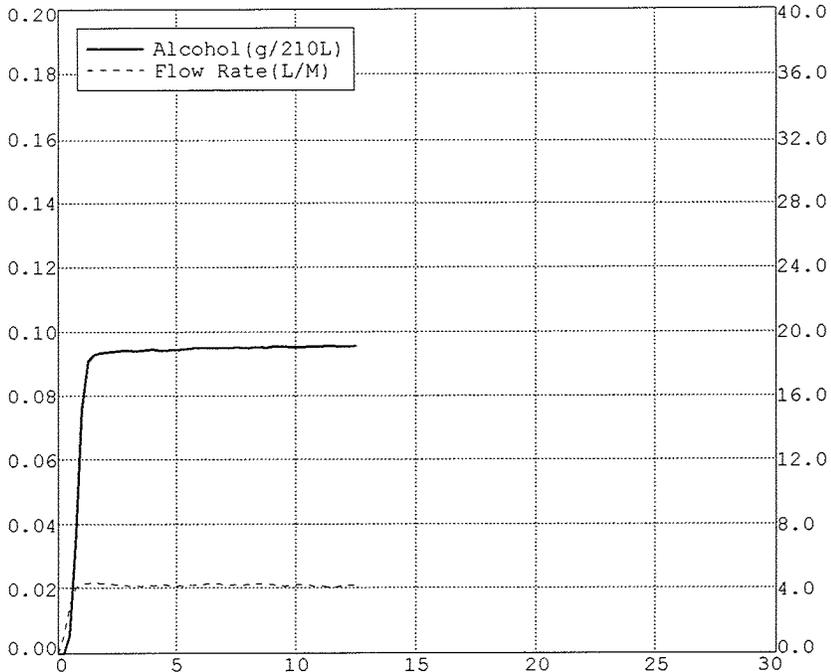

SGS RJB / Bartlett WCO #162  
 09-22-15