

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 10/06/2015

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 15180

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:06
INTERNAL STANDARD	VERIFIED	01:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:07
BLANK TEST	0.00	01:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:08
BLANK TEST	0.00	01:09
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	01:09
BLANK TEST	0.00	01:10

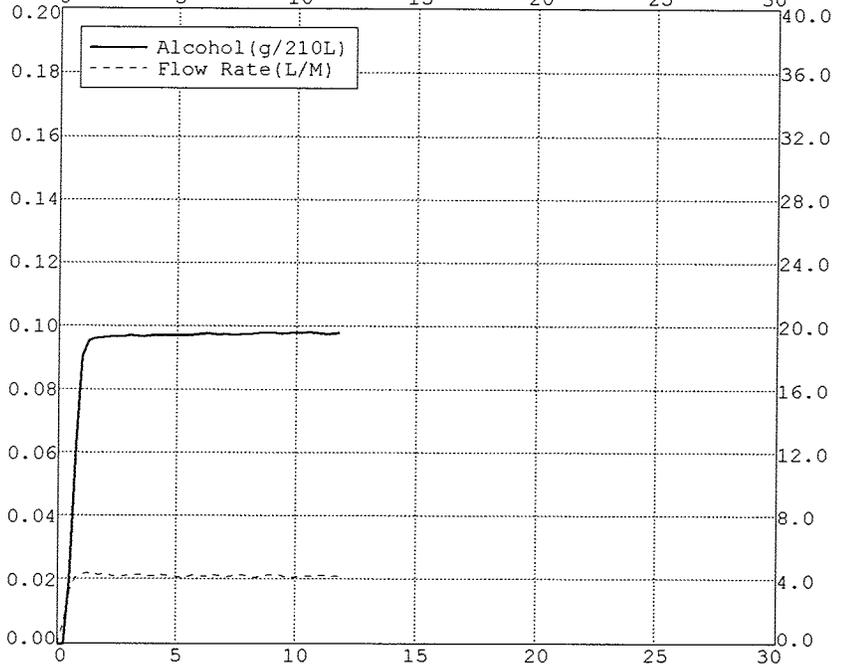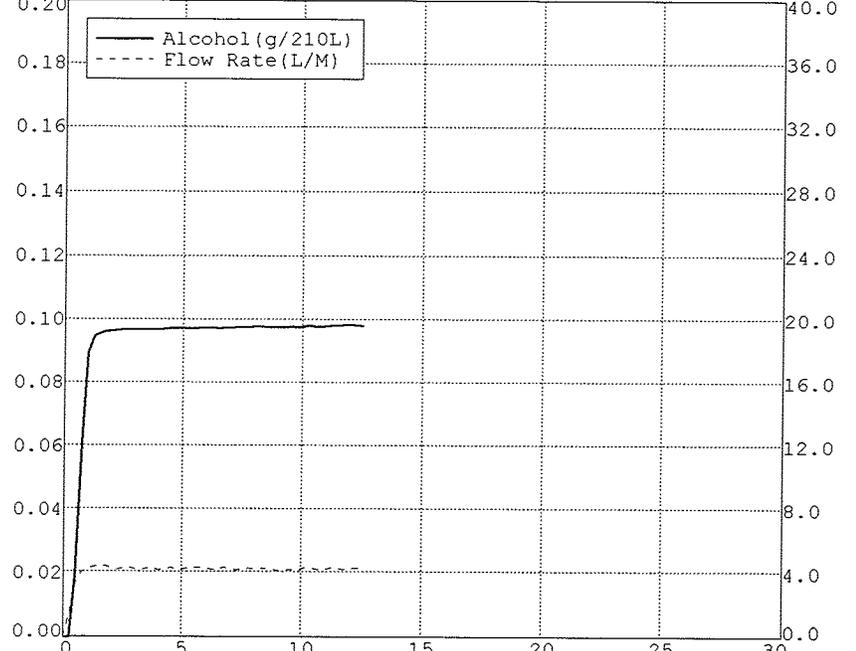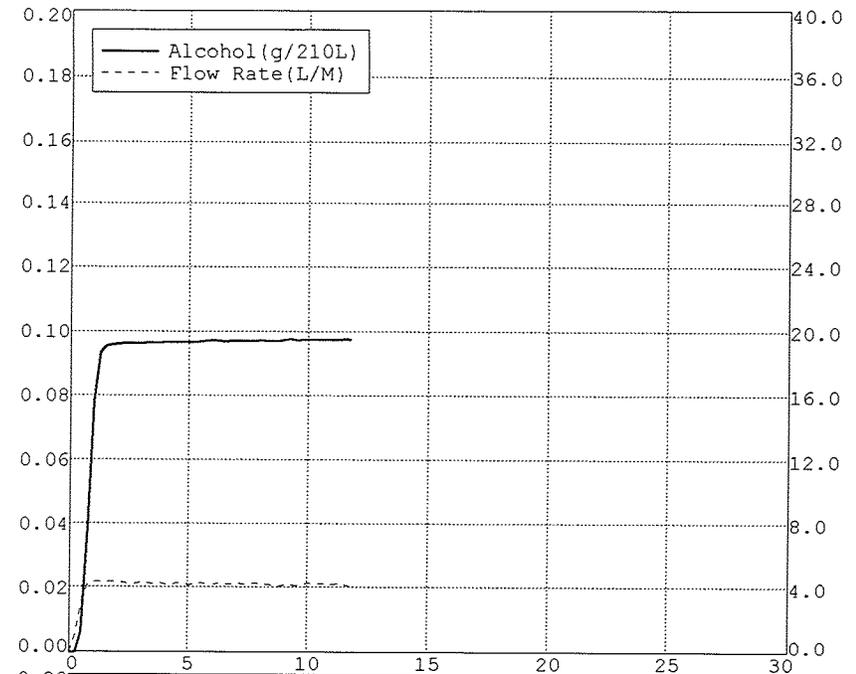

SGS B&G Bartlett W050 #142
 10-06-15