

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 11/09/2015

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 15180

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:26
INTERNAL STANDARD	VERIFIED	08:26
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	08:27
BLANK TEST	0.00	08:28
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	08:28
BLANK TEST	0.00	08:29
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	08:29
BLANK TEST	0.00	08:30

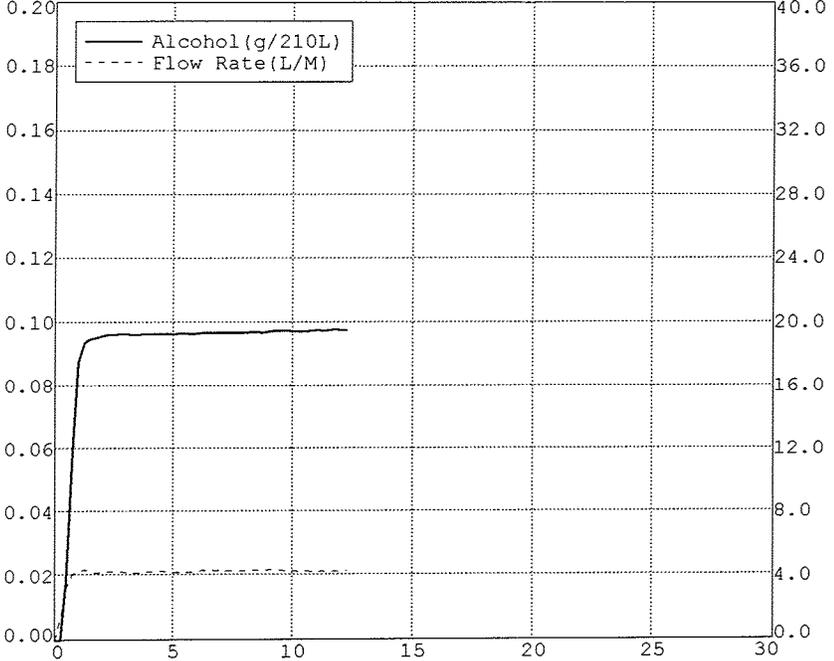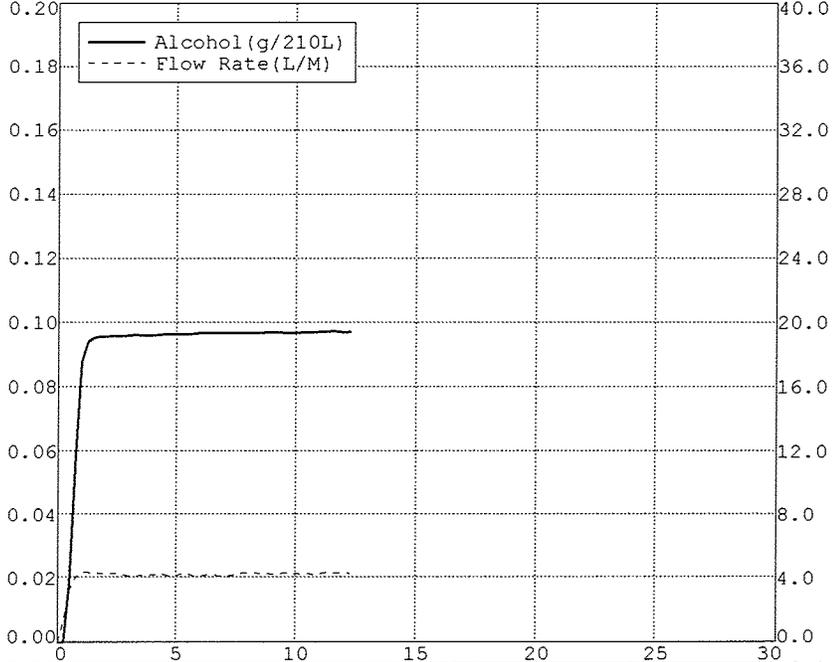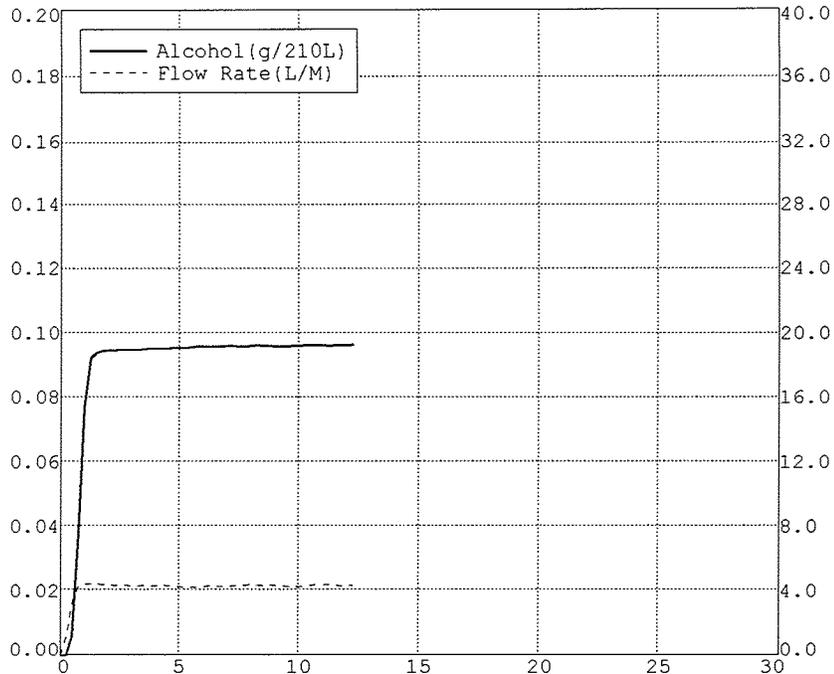

*Handwritten signature and initials*