

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 11/23/2015

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 15180

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:19
INTERNAL STANDARD	VERIFIED	12:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:20
BLANK TEST	0.00	12:20
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	12:21
BLANK TEST	0.00	12:22
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	12:22
BLANK TEST	0.00	12:23

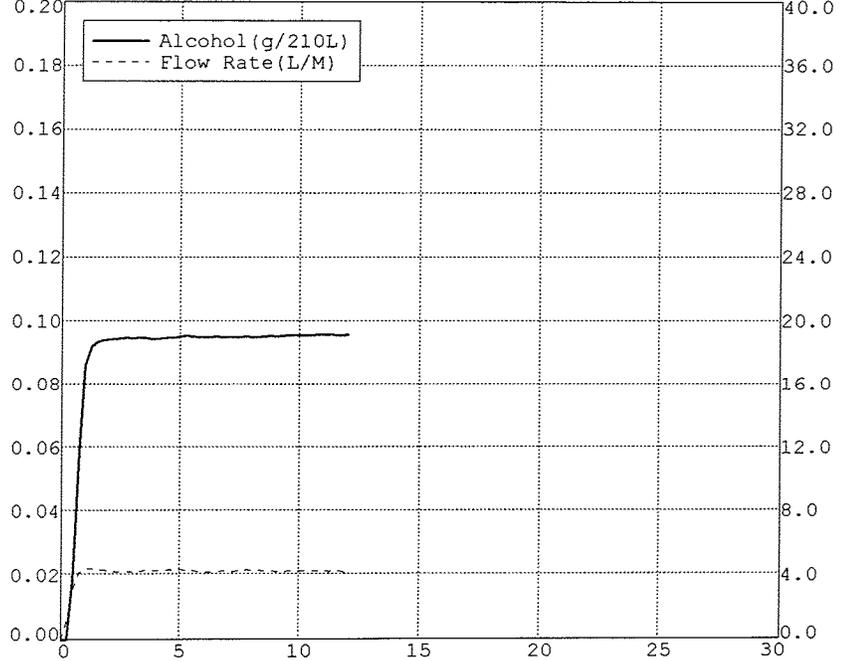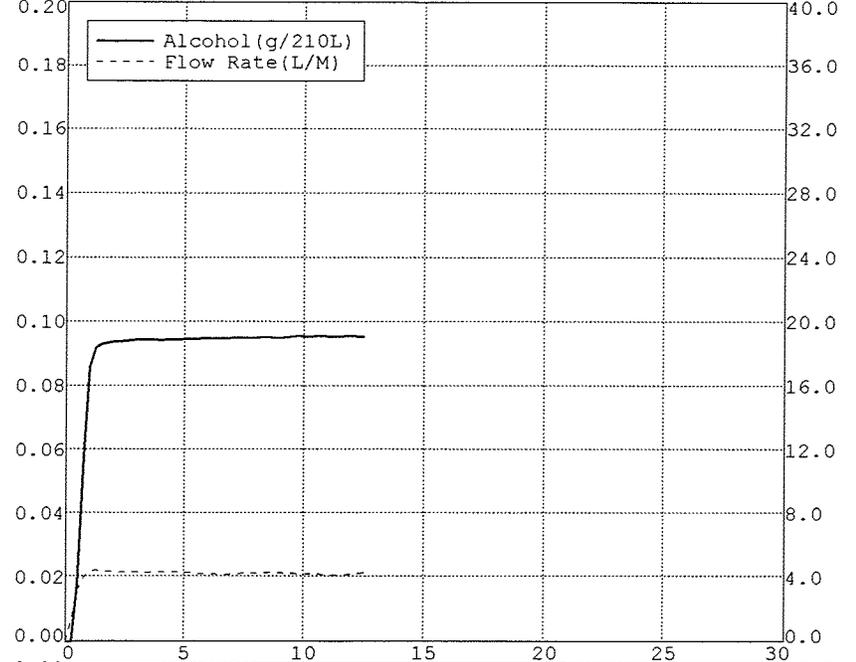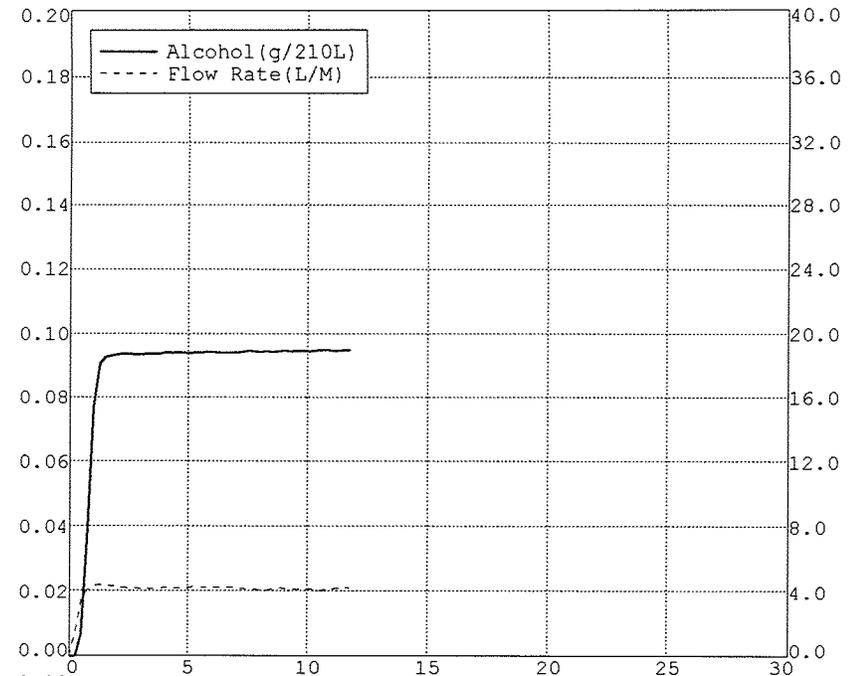

*C. B. Geisler* #248 11/23/15 1224  
HMS