

SOLUTION CHANGE




-----  
 WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 105208  
 -----

Date: 12/01/2015

OPERATOR NAME:  
 RALPH J BARTLETT  
 Permit #: 26222  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 15210

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:13
INTERNAL STANDARD	VERIFIED	00:13
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:13
BLANK TEST	0.00	00:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:15
BLANK TEST	0.00	00:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:16
BLANK TEST	0.00	00:17

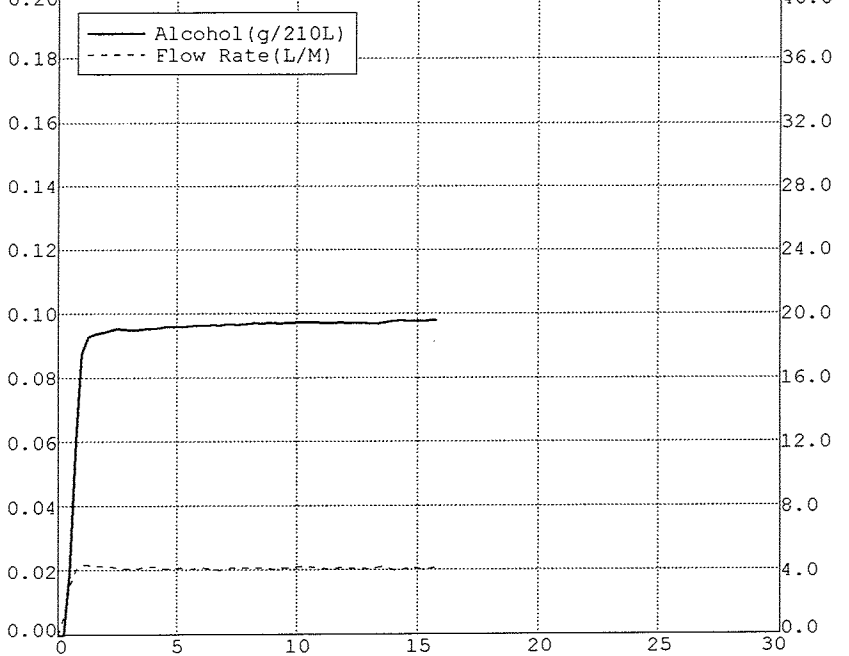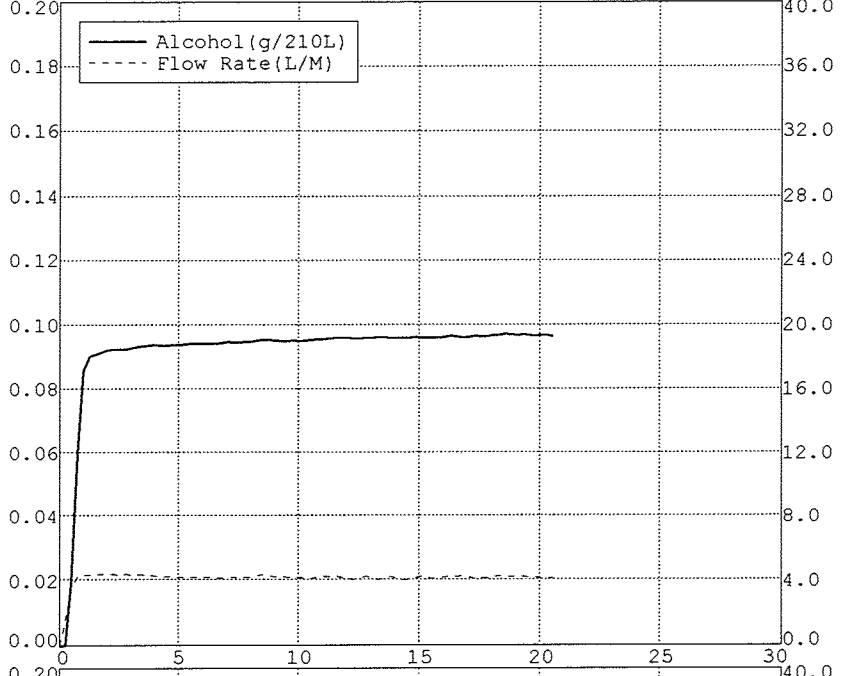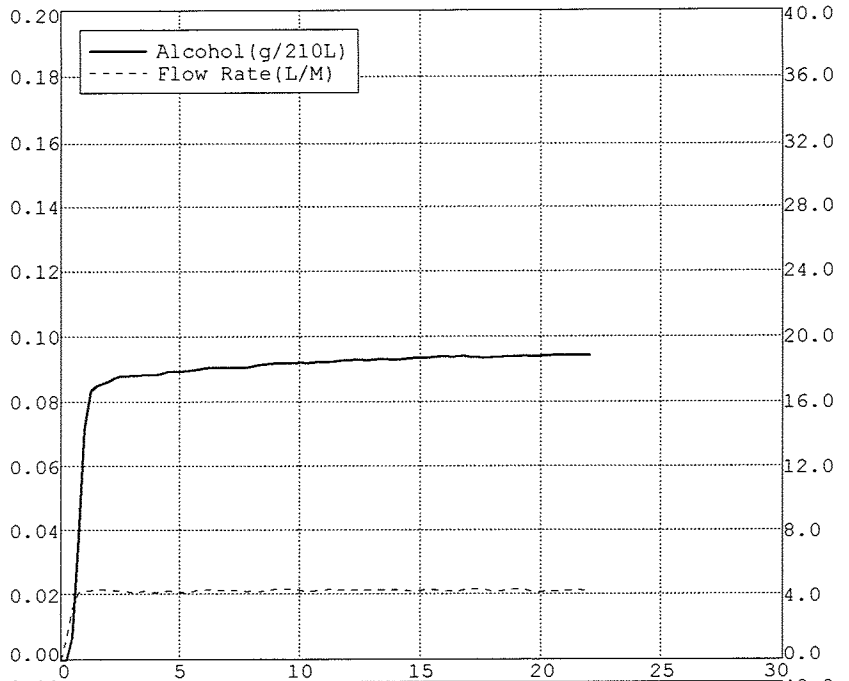

SUS Rpt / Bartlett WCSI #162  
 12-01-15