

SUPERVISOR TEST


WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 01/05/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14230

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:42
INTERNAL STANDARD	VERIFIED	01:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:42
BLANK TEST	0.00	01:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:44
BLANK TEST	0.00	01:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:45
BLANK TEST	0.00	01:46

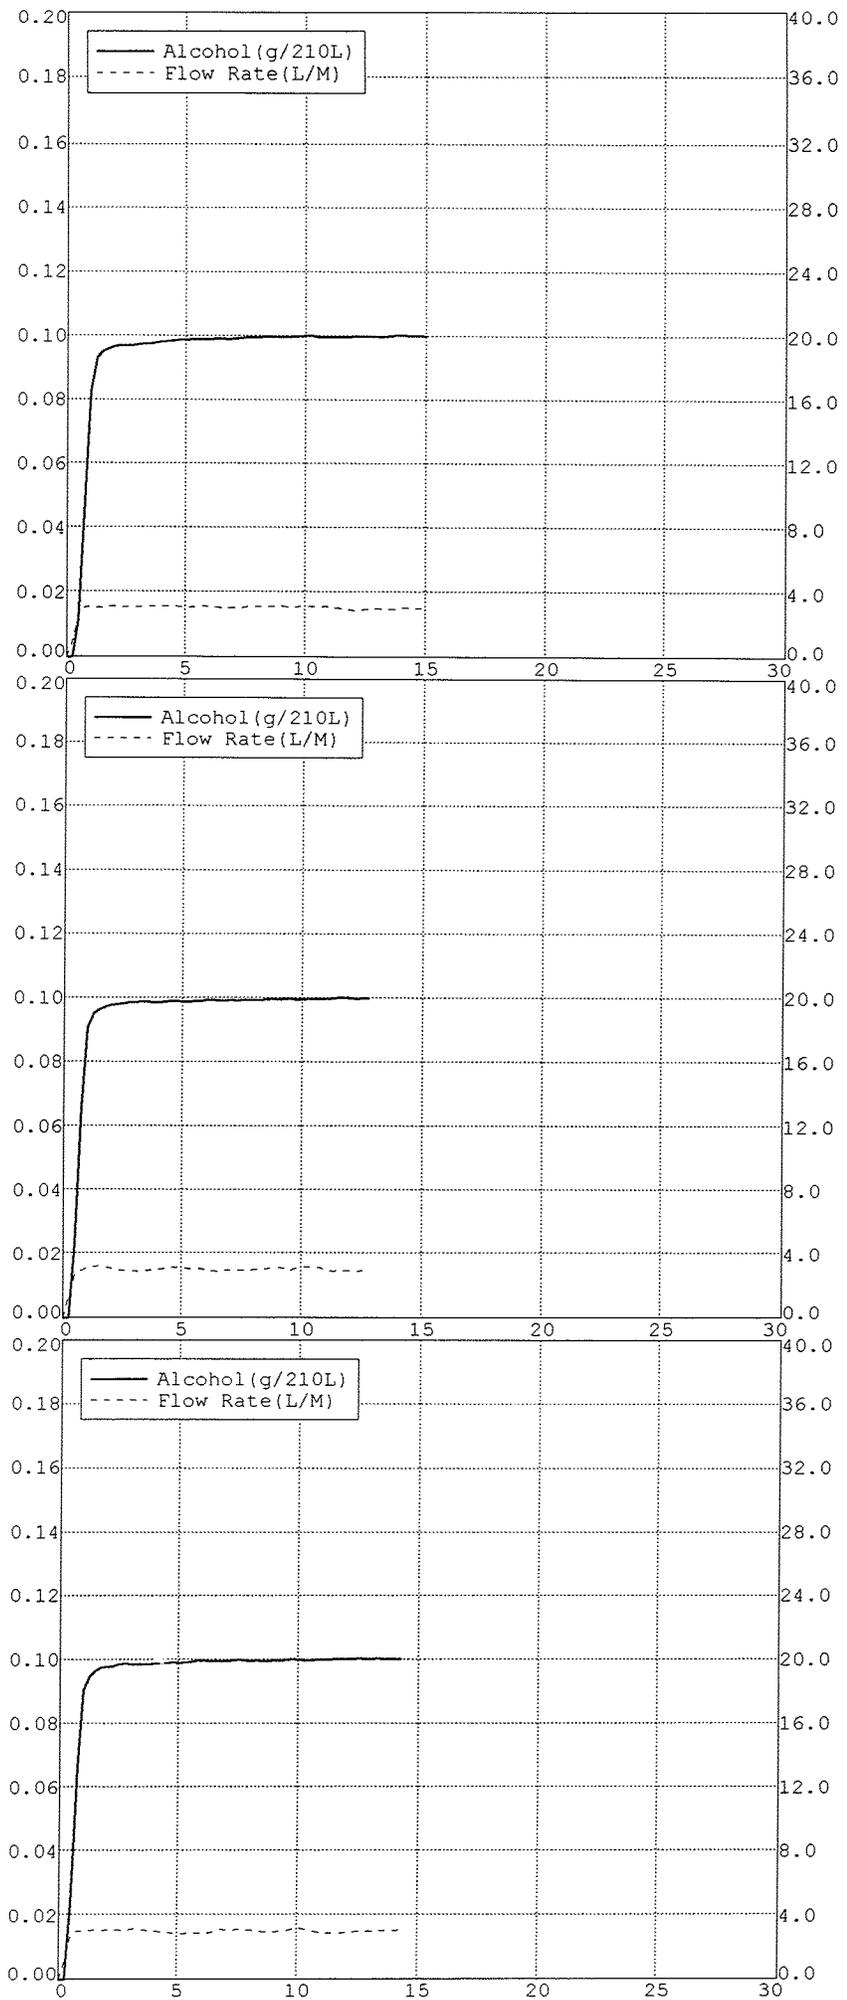

SG Bartlett WPSO #162
01-05-15