

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 01/19/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14230

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:16
INTERNAL STANDARD	VERIFIED	01:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:17
BLANK TEST	0.00	01:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:18
BLANK TEST	0.00	01:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:19
BLANK TEST	0.00	01:20

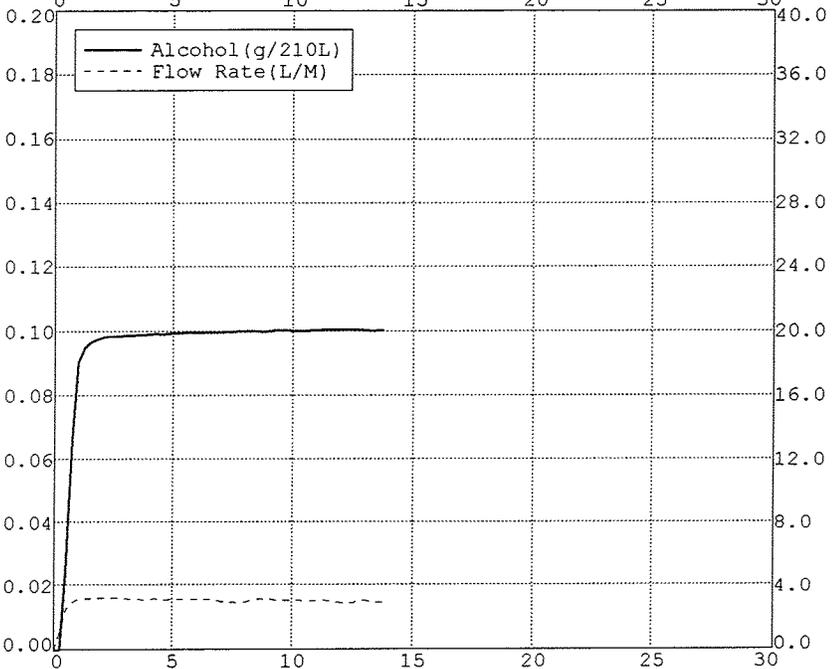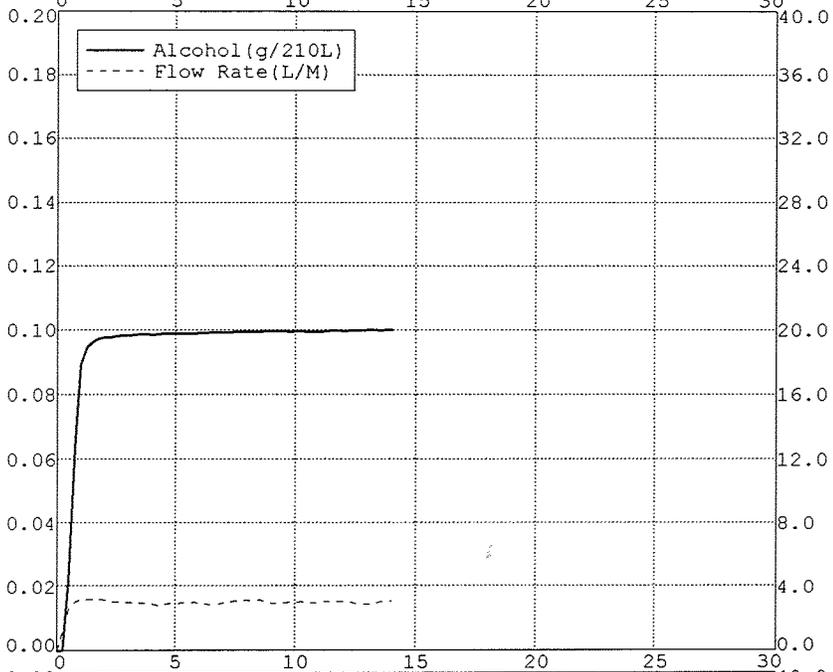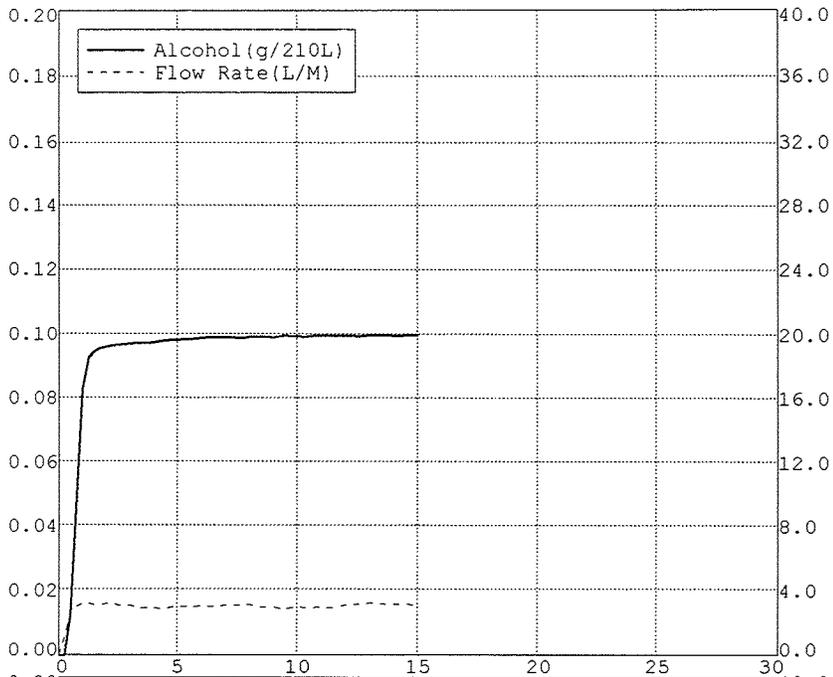

SGS RJB Bartlett W450 #162
01-19-15