

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 01/27/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14230

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:44
INTERNAL STANDARD	VERIFIED	02:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:44
BLANK TEST	0.00	02:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:45
BLANK TEST	0.00	02:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	02:47
BLANK TEST	0.00	02:48

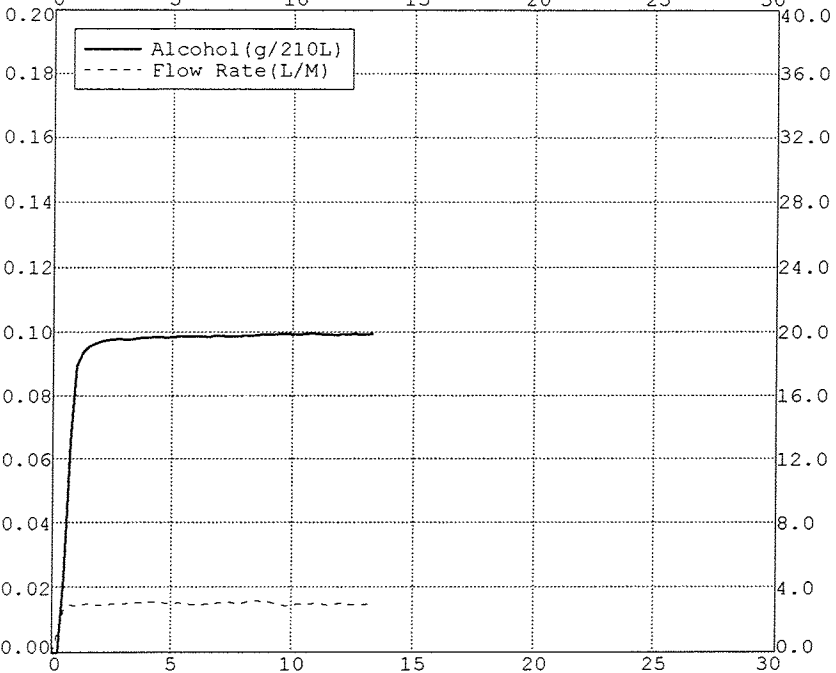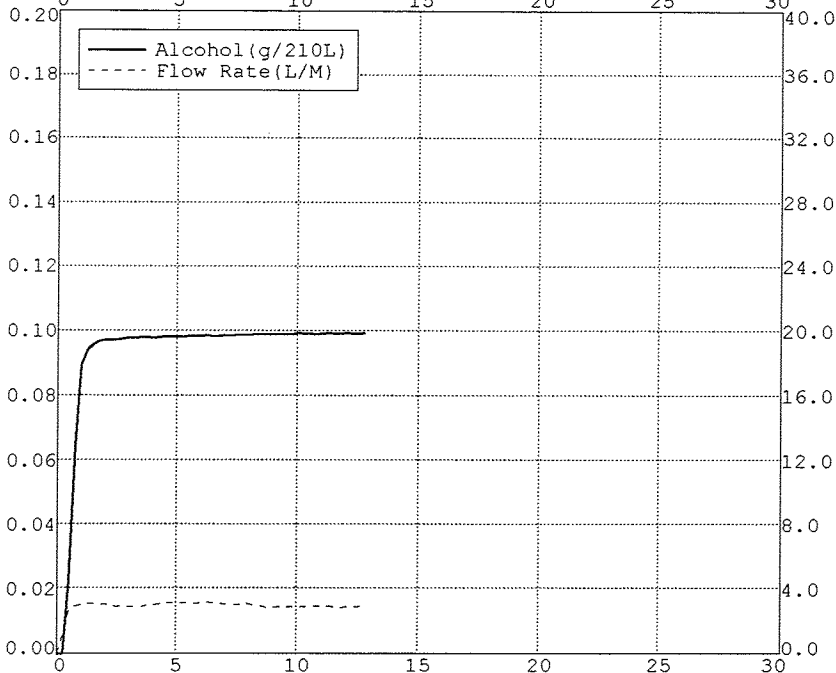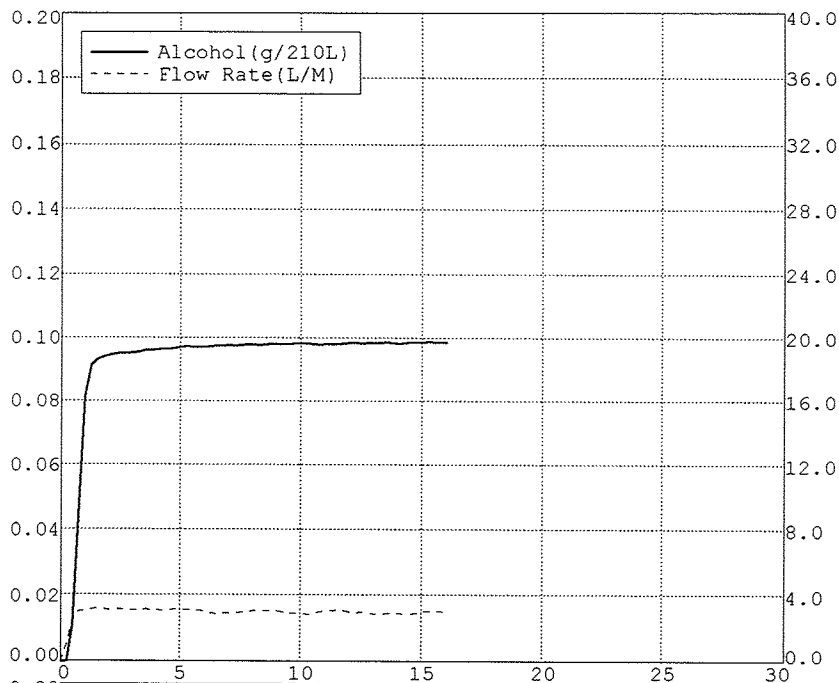

SGT R. J. Bartlett 01-27-15

SHELL #162