

SOLUTION CHANGE




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 02/02/2015

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 14260

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:34
INTERNAL STANDARD	VERIFIED	02:34
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	02:35
BLANK TEST	0.00	02:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:36
BLANK TEST	0.00	02:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:37
BLANK TEST	0.00	02:38

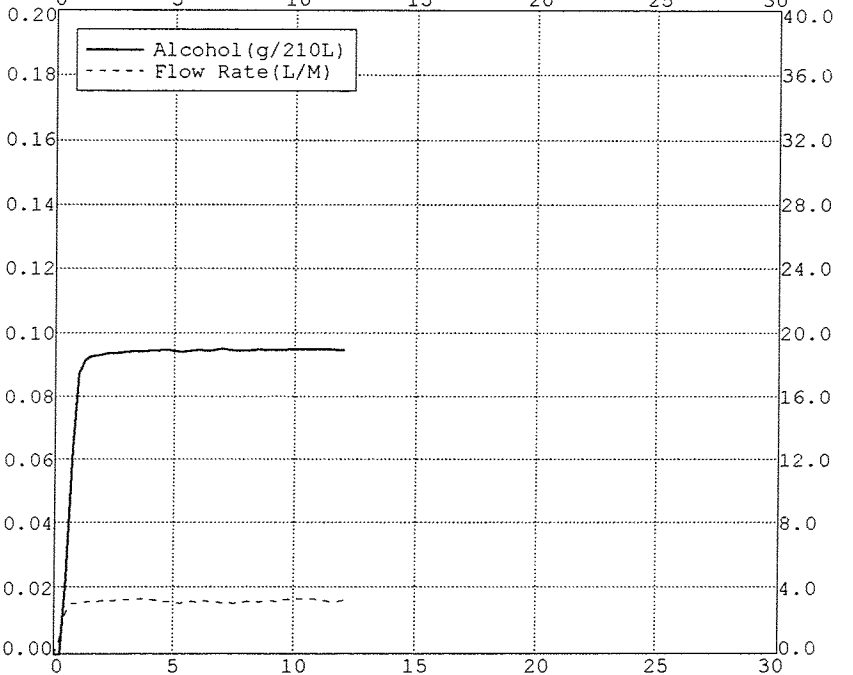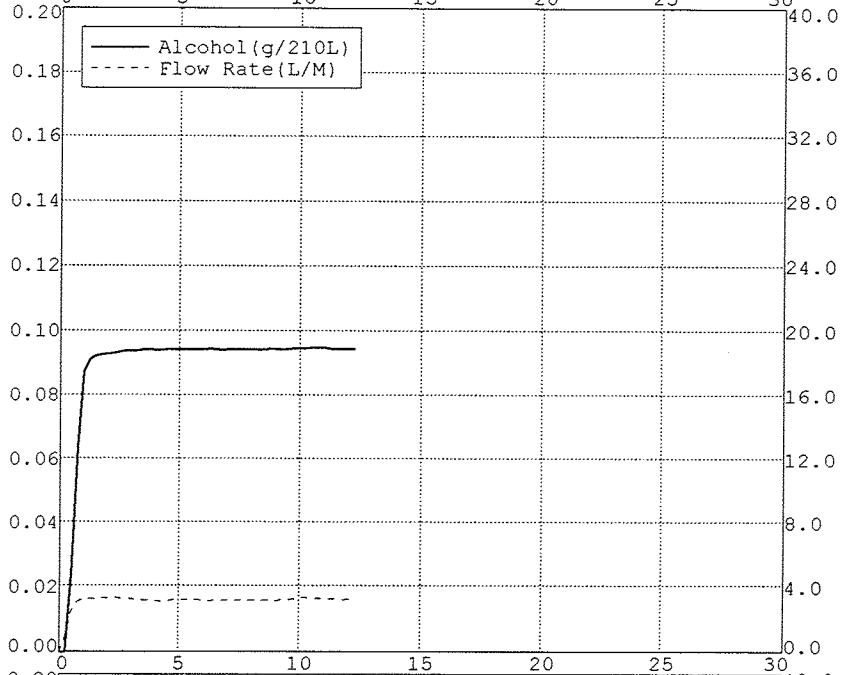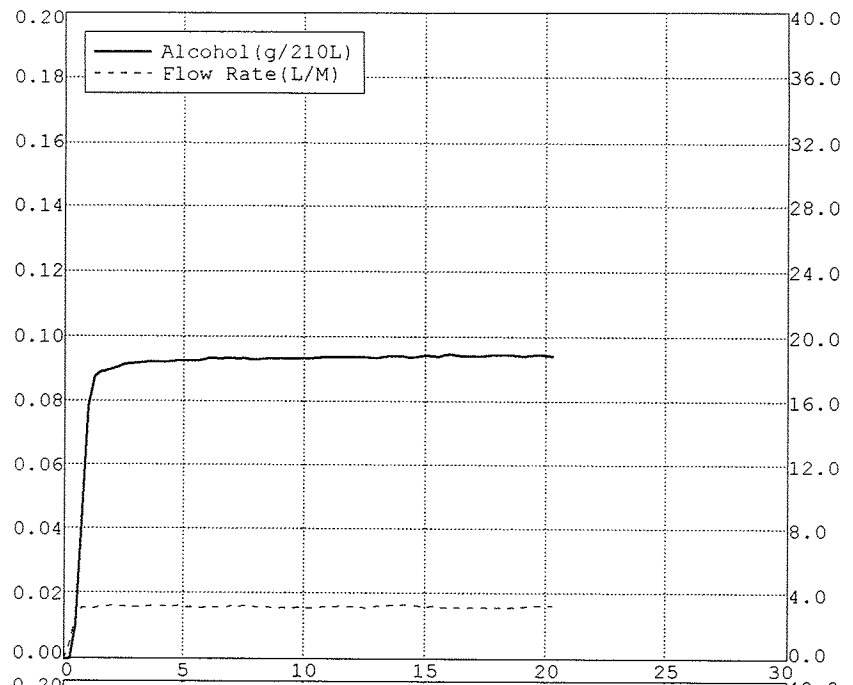

*SGS Bk / Summary w/sgu #/R
 02 02 -15*