

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 02/24/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14260

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:04
INTERNAL STANDARD	VERIFIED	02:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:04
BLANK TEST	0.00	02:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:06
BLANK TEST	0.00	02:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:07
BLANK TEST	0.00	02:08

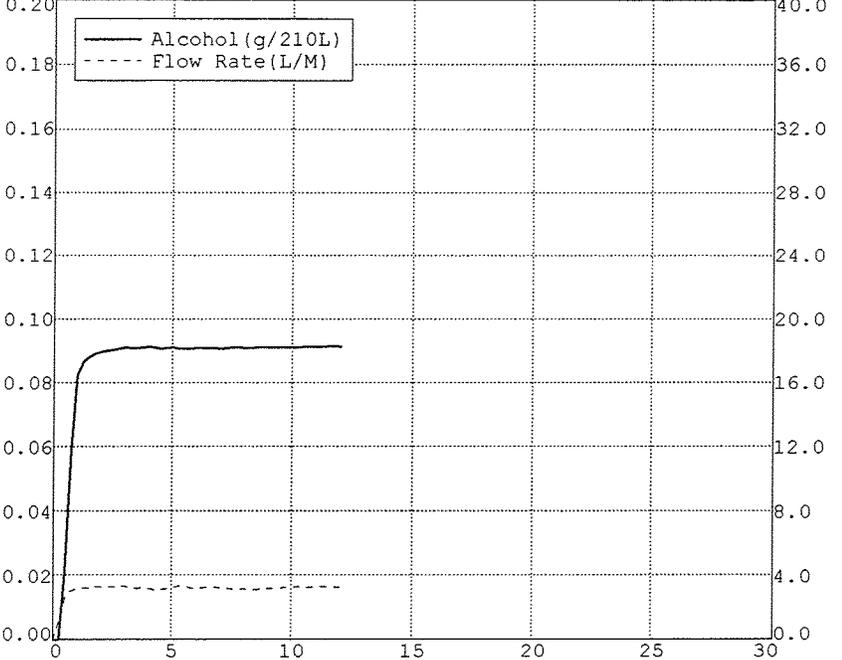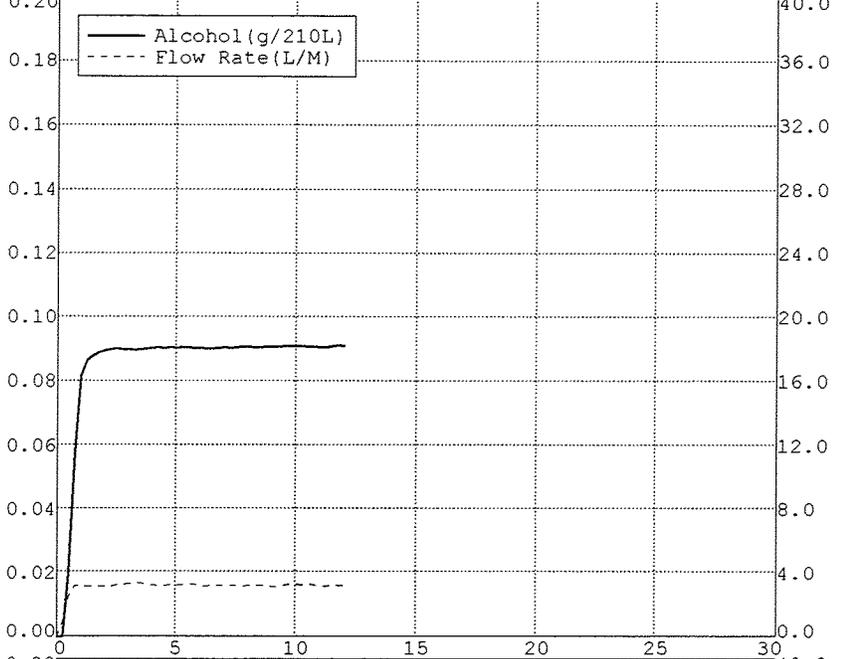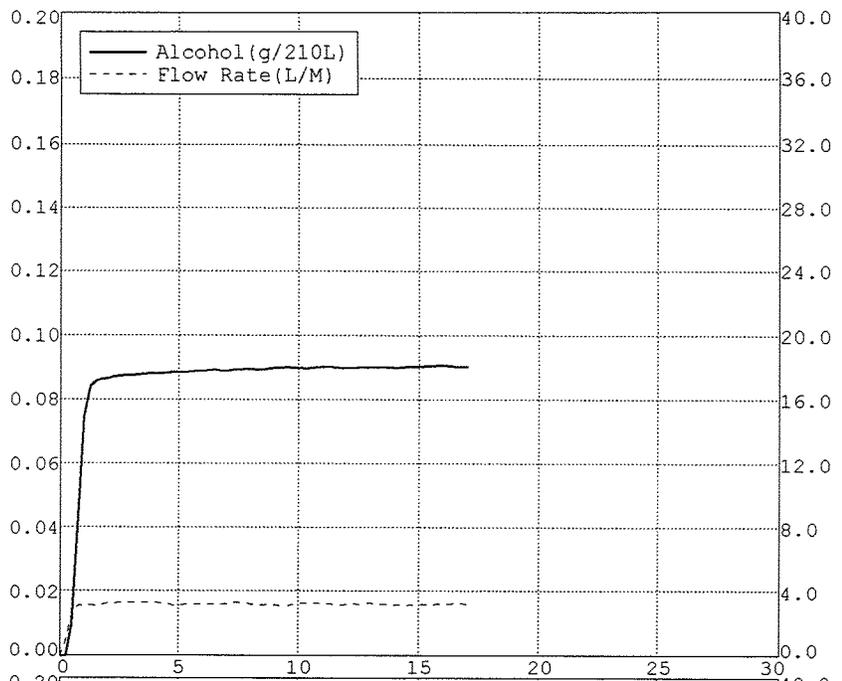

SGS Ralph Bartlett WOSO #162
02-24-15