

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 03/10/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 14260

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:07
INTERNAL STANDARD	VERIFIED	01:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:07
BLANK TEST	0.00	01:08
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	01:08
BLANK TEST	0.00	01:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:09
BLANK TEST	0.00	01:10

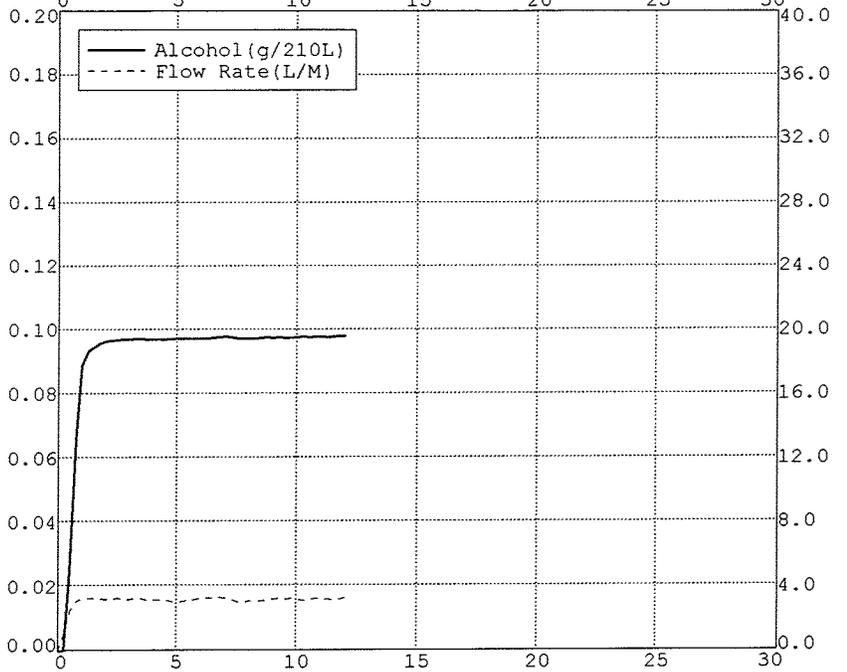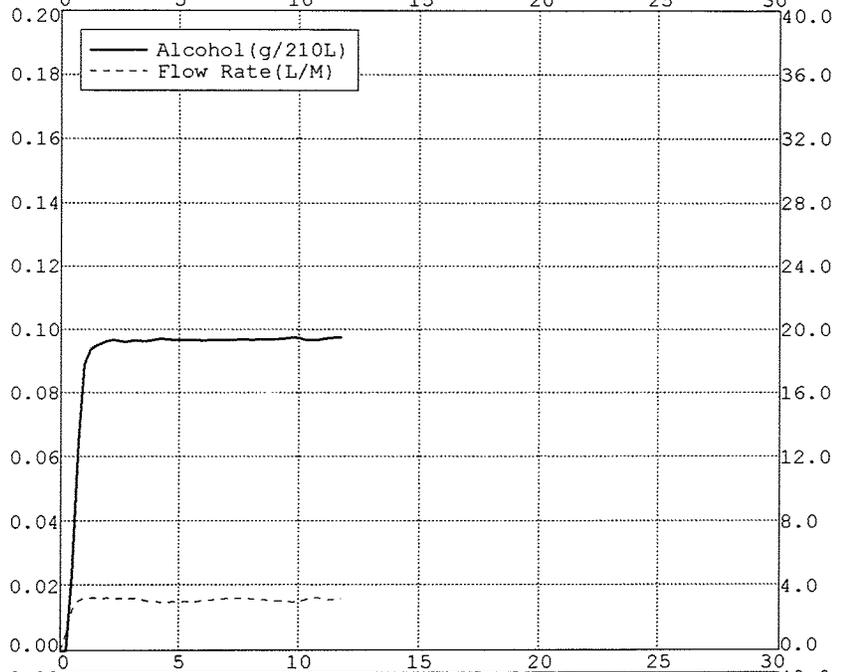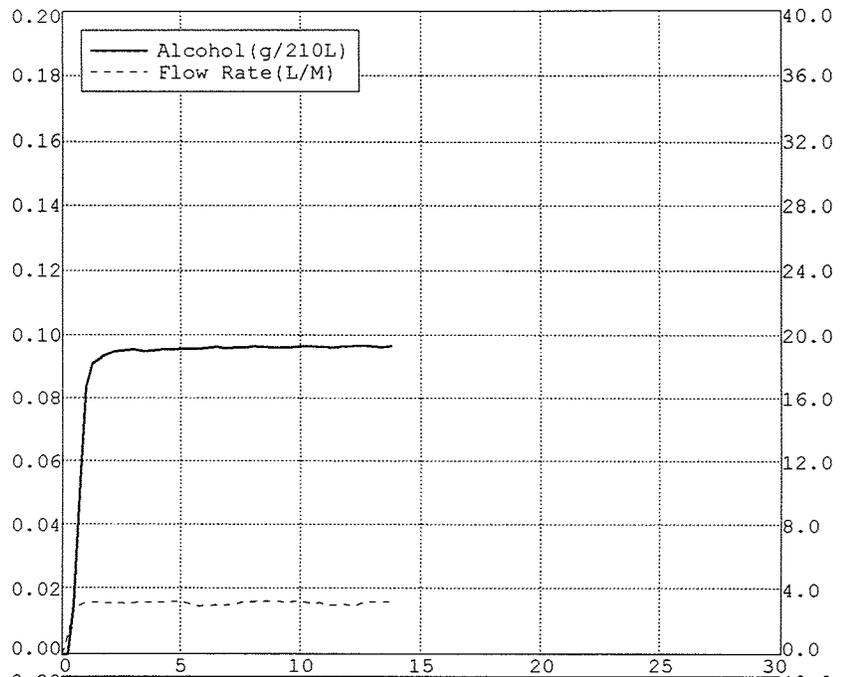

SGS RJB Bartlett
WCSO #162 03-10-15