

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 03/16/2015

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 14260

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:47
INTERNAL STANDARD	VERIFIED	02:47
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:47
BLANK TEST	0.00	02:48
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:48
BLANK TEST	0.00	02:49
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:50
BLANK TEST	0.00	02:51

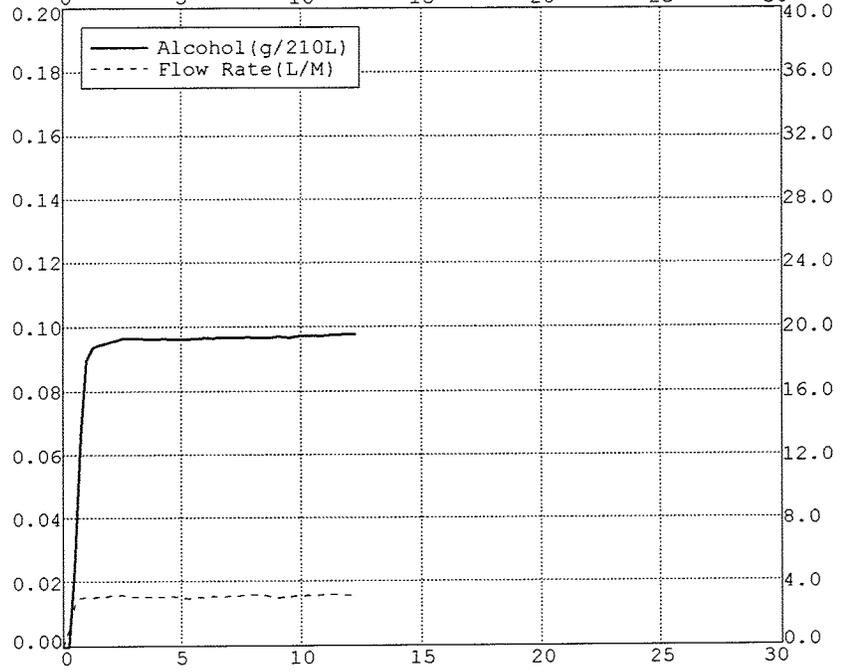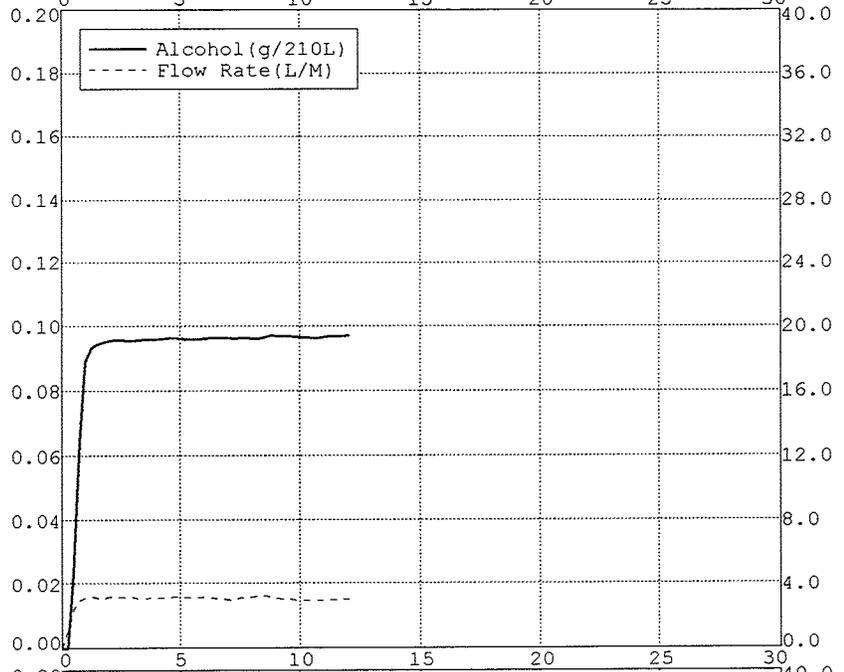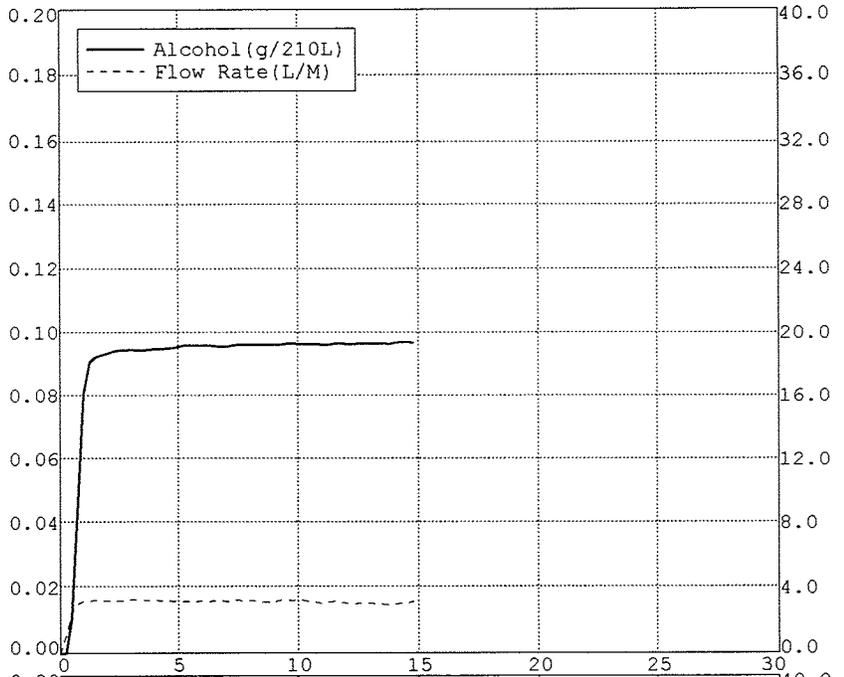

*SOS Rly Bureaus w/eso #162*  
*03-16-15*