

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 04/13/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15010

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:39
INTERNAL STANDARD	VERIFIED	01:39
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:40
BLANK TEST	0.00	01:41
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	01:41
BLANK TEST	0.00	01:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:42
BLANK TEST	0.00	01:43

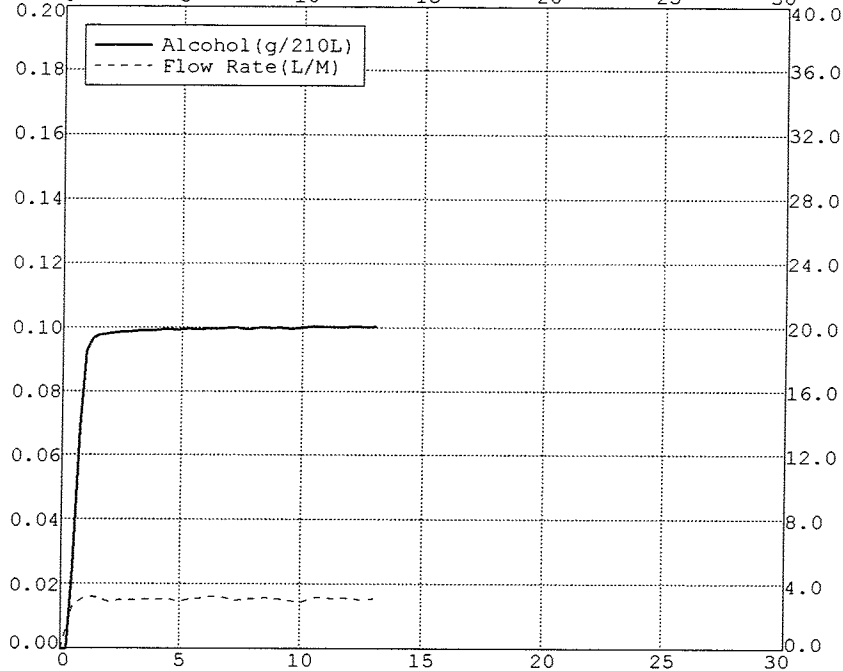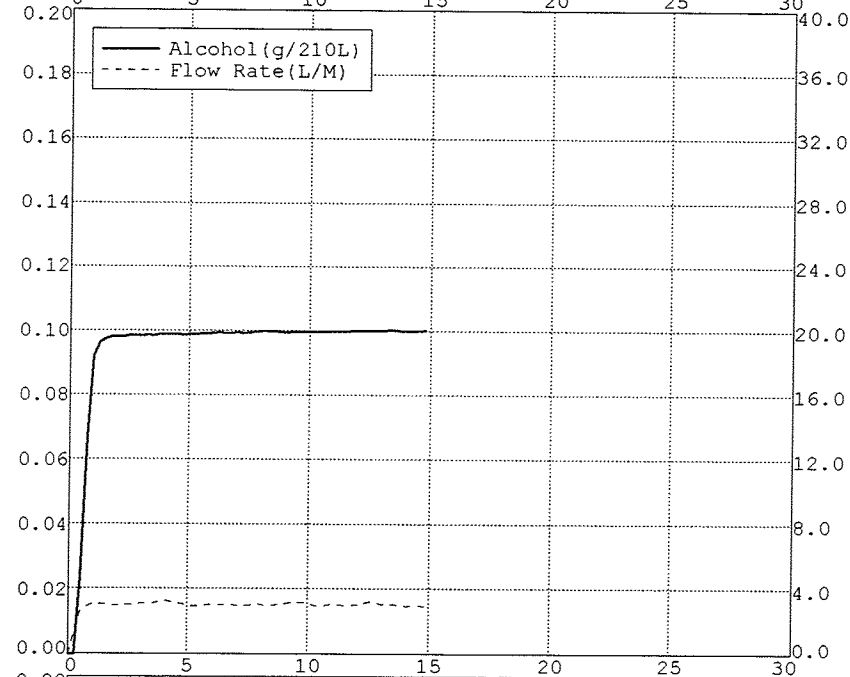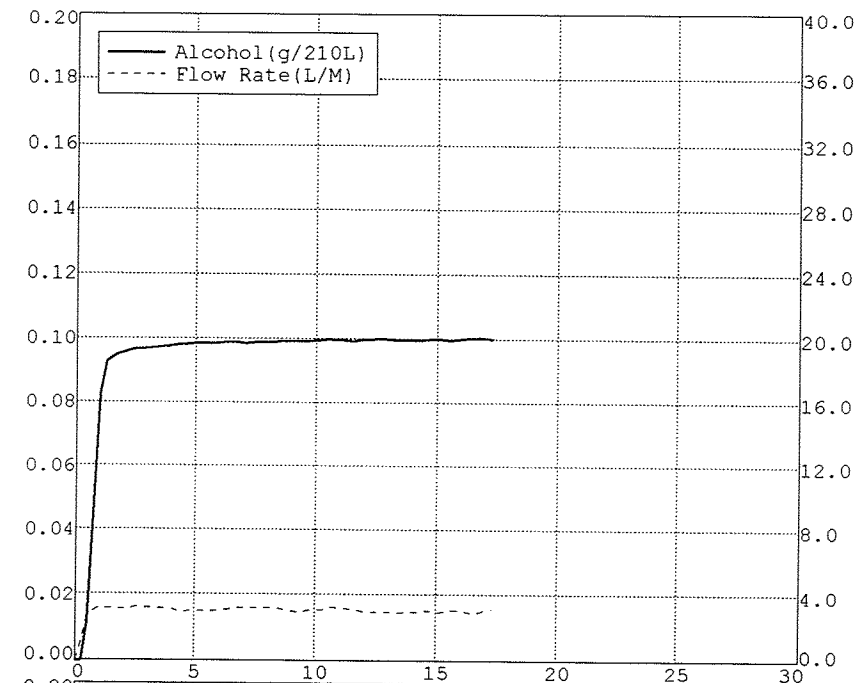

SGS *RJ Bartlett*
werc #162 04/13/15