

SUPERVISOR TEST




-----  
 WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 106606  
 -----

Date: 04/27/2015

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 15010

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:55
INTERNAL STANDARD	VERIFIED	07:55
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	07:55
BLANK TEST	0.00	07:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:56
BLANK TEST	0.00	07:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:58
BLANK TEST	0.00	07:58

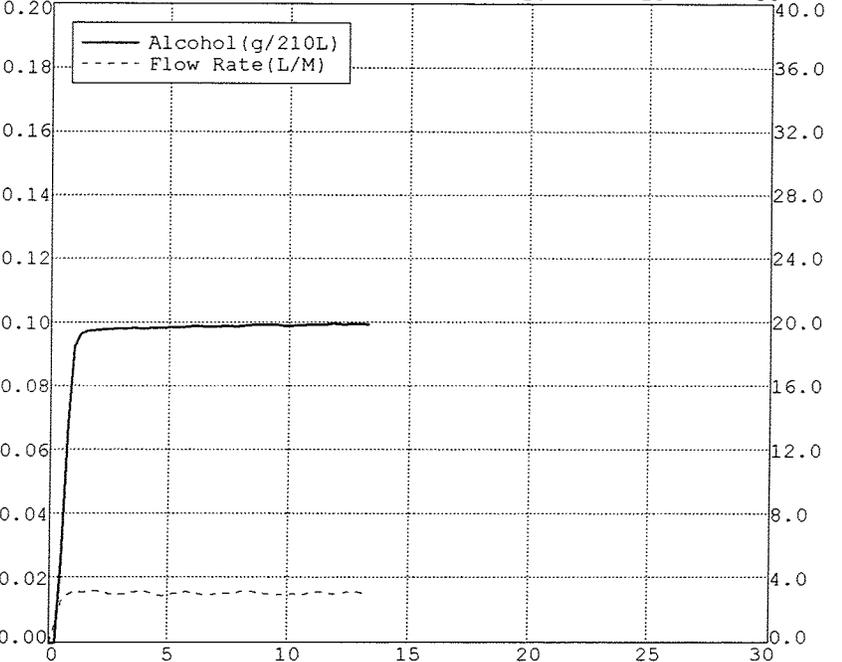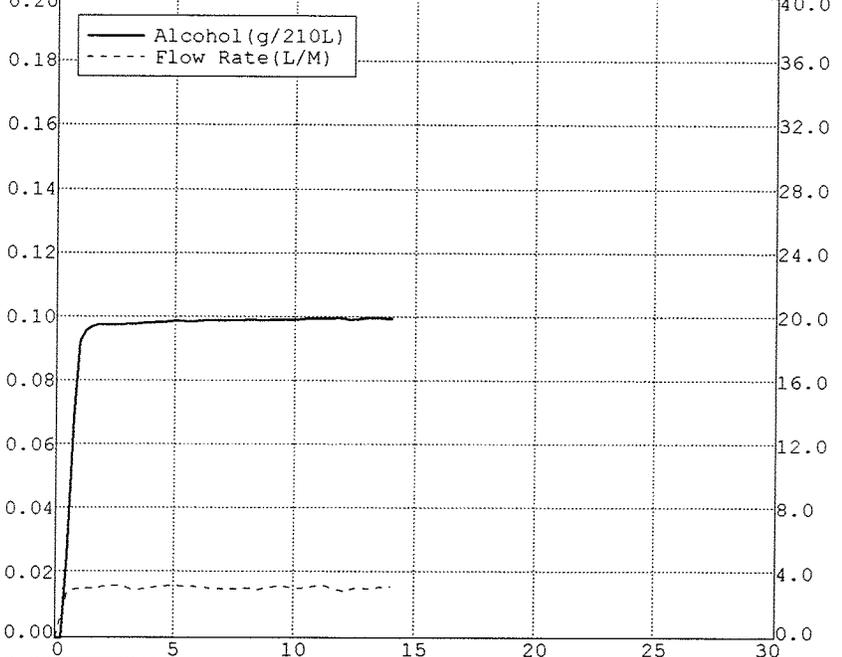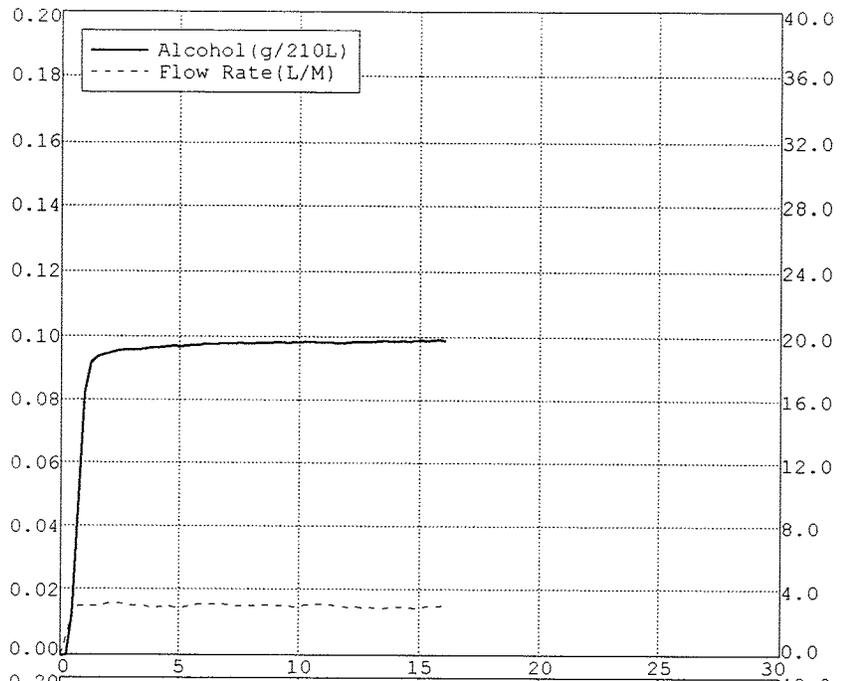

*J. A. G. #242*