

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 05/13/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15010

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:35
INTERNAL STANDARD	VERIFIED	11:35
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	11:35
BLANK TEST	0.00	11:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:36
BLANK TEST	0.00	11:37
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:37
BLANK TEST	0.00	11:38

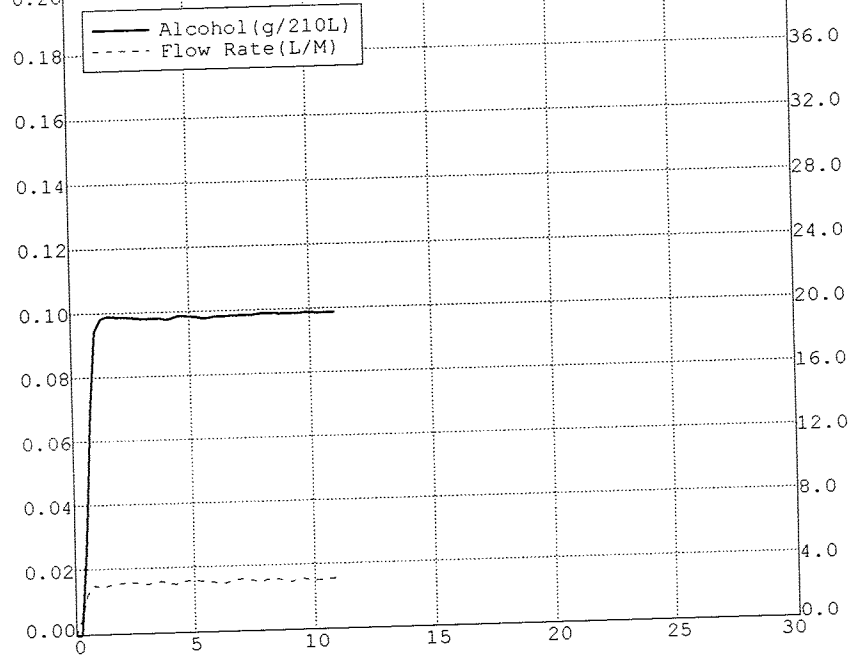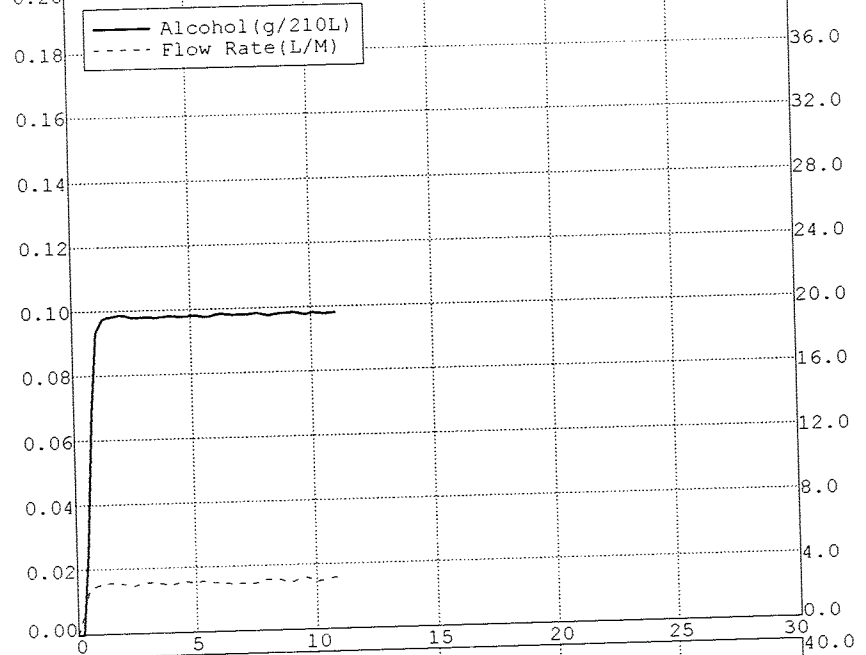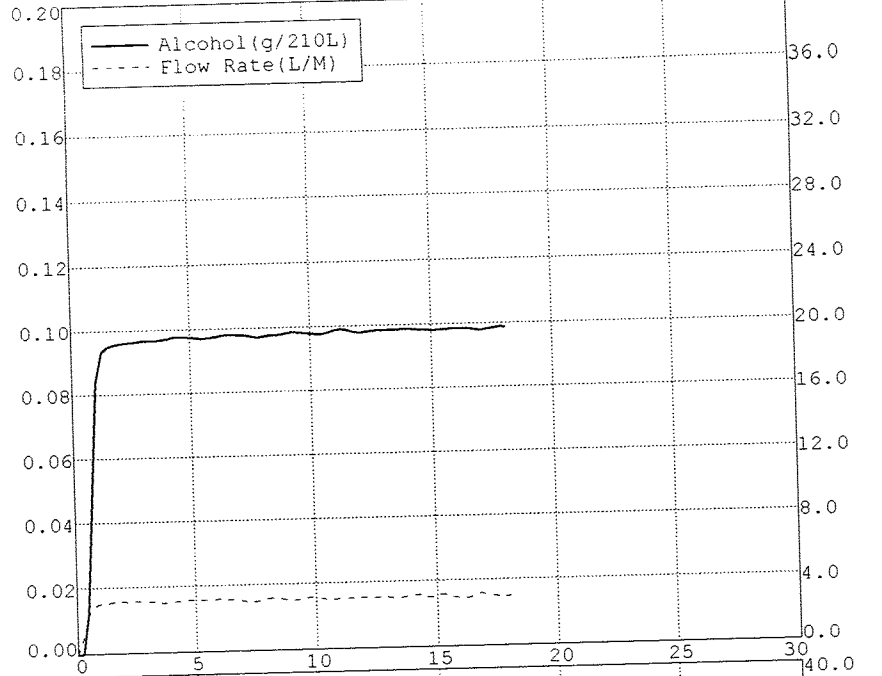

565 RJA Run w/ser #102
05-04-15