

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 05/18/2015

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15010

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:55
INTERNAL STANDARD	VERIFIED	14:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:56
BLANK TEST	0.00	14:57
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	14:57
BLANK TEST	0.00	14:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:58
BLANK TEST	0.00	14:59

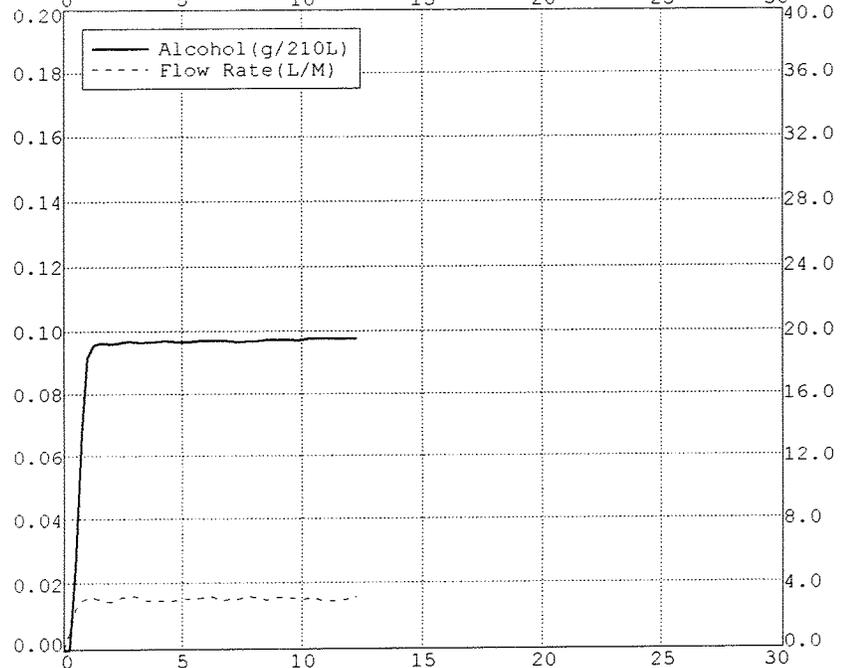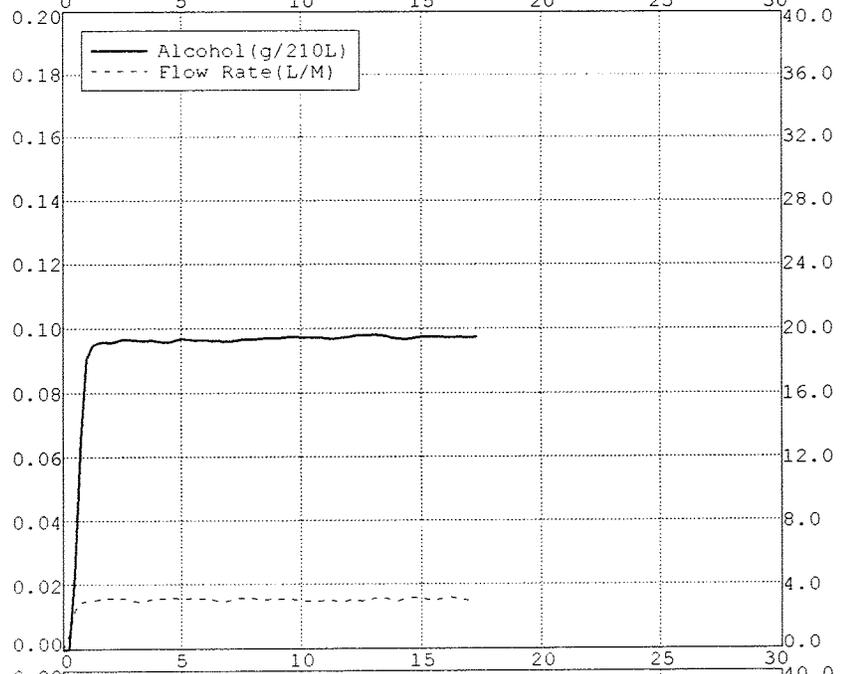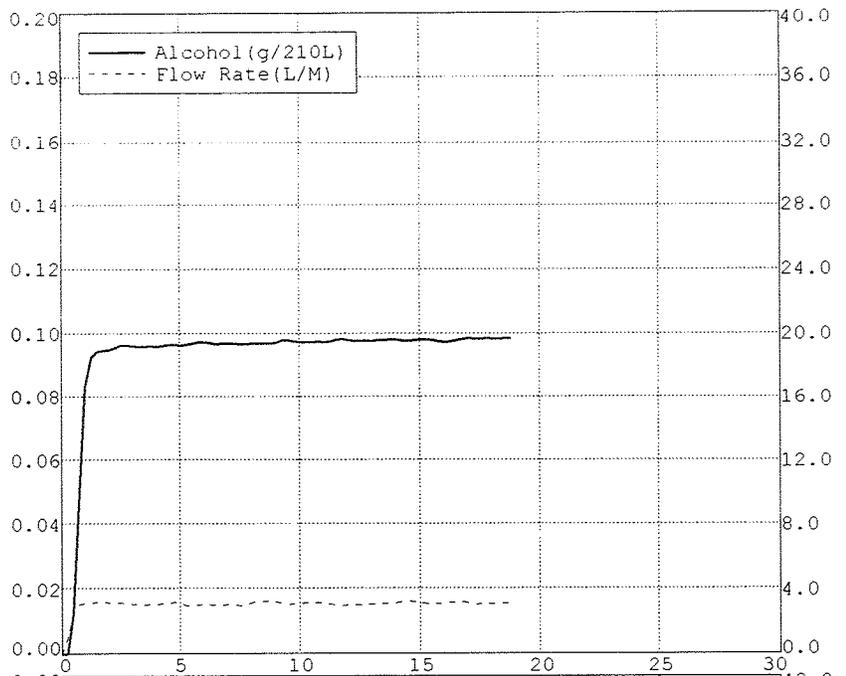

SGS RJB Bartlett #162

05-18-15