

SUPERVISOR TEST




 WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 06/16/2015

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 15070

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:06
INTERNAL STANDARD	VERIFIED	04:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	04:06
BLANK TEST	0.00	04:07
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	04:07
BLANK TEST	0.00	04:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	04:09
BLANK TEST	0.00	04:09

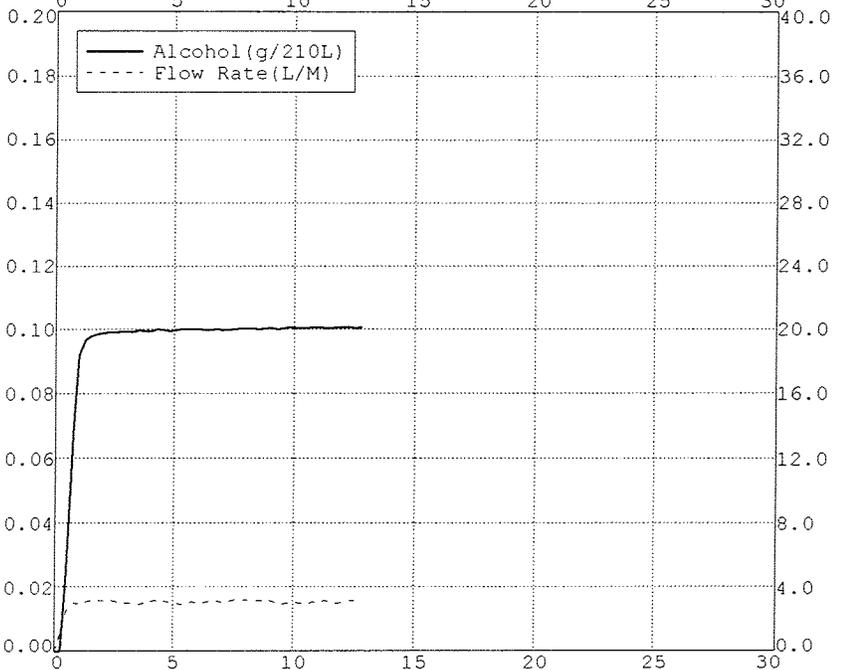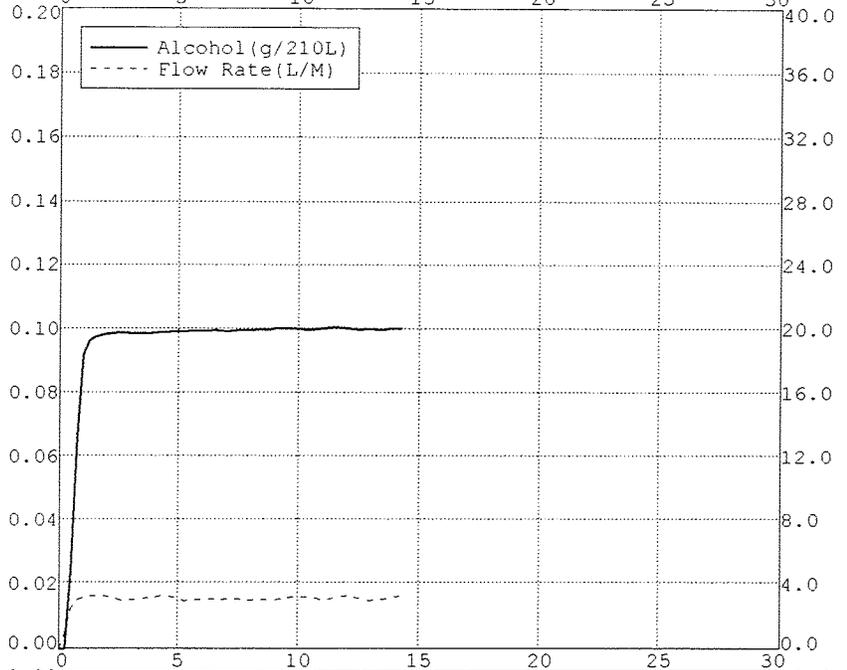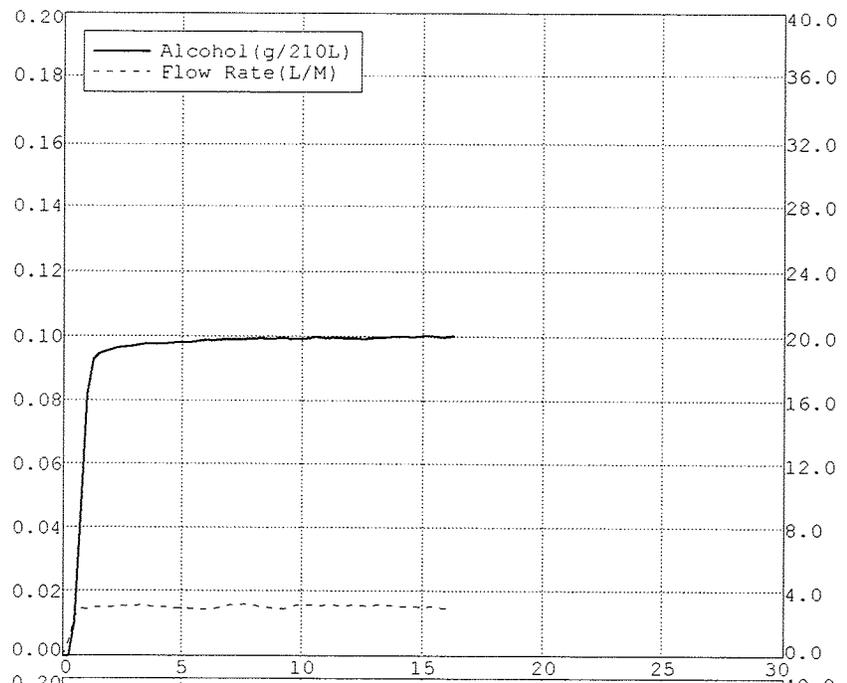

SG RJB / Bartlett WCO #102
06/16/15